


 Cite this: *RSC Adv.*, 2023, 13, 24777

Construction of an optical sensor for copper determination in environmental, food, and biological samples based on the covalently immobilized 2-(2-benzothiazolylazo)-3-hydroxyphenol in agarose

 Mai Aish,^a Reem F. Alshehri^b and Alaa S. Amin *^c

An optical chemical sensor has been developed for the quantitative spectrophotometric analysis of copper. The optode is dependent on covalent immobilization of 2-(2-benzothiazolylazo)-3-hydroxyphenol (BTAHP) in a transparent agarose membrane. The absorbance variation of immobilized BTAHP on agarose as a film upon the addition of 5×10^{-3} M aqueous solutions of Mn^{2+} , Zn^{2+} , Hg^{2+} , Cd^{2+} , Pb^{2+} , Co^{2+} , Ni^{2+} , Fe^{2+} , La^{3+} , Fe^{3+} , Cr^{3+} , Zr^{4+} , Se^{4+} , Th^{4+} , and UO_2^{2+} revealed substantially higher changes in the Cu^{2+} ion content compared to other ions investigated here. The effects of various experimental parameters, such as the solution pH, the reaction time, and the concentration of reagents, on the quality of Cu^{2+} sensing were examined. Under ideal experimental circumstances, a linear response was achieved for Cu^{2+} concentrations ranging from 1.0×10^{-9} to 7.5×10^{-6} M with an R^2 value of 0.9988. The detection (3σ) and quantification (10σ) limits of the procedure for Cu^{2+} analyses were 3.0×10^{-10} and 9.8×10^{-10} M, respectively. No observable interference was recorded in the detection of Cu^{2+} due to other inorganic cations. With no indication of BTAHP leaching, the membrane demonstrated good durability and quick response times. The optode was effectively used to determine the presence of Cu^{2+} in environmental water, food, and biological samples.

 Received 25th June 2023
 Accepted 6th August 2023

DOI: 10.1039/d3ra04249a

rsc.li/rsc-advances

Introduction

Heavy metal pollution is a severe global environmental problem due to its impacts, such as genetic alteration in all living things. Currently, efforts to eliminate this hazardous material have accelerated. Technology advancement and rapid industrialization have enhanced the need for high-purity materials. Trace element measurements are becoming much more crucial because of how such elements affect human metabolism.¹

The most important trace element in the human body, *i.e.*, copper, comes in third place in terms of abundance.² In actuality, the liver comes in second place to the brain in terms of copper content.³ This abundance is attributable to the important functions that copper ions play in a wide range of biological activities, including neuromodulation, antioxidative defense, and response to hypoxia.⁴

Due to its redox-active nature, copper is a well-known important trace mineral for organisms and is crucial for many

key physiological processes in the human body.^{5–9} Cu^{2+} is frequently utilized as an auxiliary ion in reactions that are catalyzed by enzymes because of its powerful coordination ability. The unsuitable concentration of Cu^{2+} in the body, however, is the cause of several diseases, including Wilson's, Alzheimer's, Menkes, Prion, and Huntington's diseases, *etc.* Cu^{2+} is second only to mercury in drinking water in terms of toxicity.^{10–17}

The accumulation of copper ions occurs when people and animals are exposed to excessive amounts of Cu^{2+} -contaminated water, and thus, it is hazardous to the environment and ecosystem and can also affect the progression of diseases, such as Alzheimer's and Parkinson's.^{10,18,19} Additionally, Cu^{2+} , which has a very harmful effect on aquatic creatures, is a frequent environmental pollutant in aquaculture systems.²⁰ A tolerable amount of Cu^{2+} in drinking water has been determined to be between 25 and 31.5 μM by the World Health Organization (WHO) and the U.S. Environmental Protection Agency (EPA), respectively.²¹ Consequently, simple, practical, and affordable Cu^{2+} sensor technologies must be developed to successfully detect and monitor its content in drinking water, food, industrial processes, and biological systems. This will help overcome the problem of Cu^{2+} playing a crucial role in both the

^aChemistry Department, Faculty of Science, Port Said University, Port Said, Egypt. E-mail: asamin2005@hotmail.com
^bChemistry Department, College of Science, Taibah University, Madina, Kingdom of Saudi Arabia

^cChemistry Department, Faculty of Science, Benha University, Benha, Egypt


environment and the human body. Developing colorimetric sensors for the detection of Cu²⁺ is particularly important.

To detect Cu²⁺ ions at a trace level, several instrumental analytical chemistry methods can be utilized in the lab, such as spectrophotometry,²² fluorometry,^{23,24} atomic absorption spectroscopy (AAS),^{25–28} inductively coupled plasma-atomic emission spectroscopy (ICP-AES),^{29–32} inductively coupled plasma-mass spectrometry (ICP-MS),^{33,34} laser-induced breakdown spectroscopy (LIBS),³⁵ and anodic stripping voltammetry.^{36–38} These instrumental methods have some limitations despite having a good limit of detection (LOD) and a wider working concentration range, such as a long and tedious analysis time, the need for expensive and sophisticated equipment, a difficult sample pre-treatment procedure, and unreliable capabilities for *in situ* analysis.^{39–42} Therefore, the need to develop portable, user-friendly tools for efficient and precise screening of Cu²⁺ ions has gained increasing interest. To determine the presence of the Cu²⁺ ion using electrochemical methods, such as potentiometric and amperometric methods, selective electrodes are required to eliminate the possibility of interference from other ions.^{43,44} On the other hand, chemical sensors based on optical transducers, for example, UV-Vis spectrophotometers have shown the potential to achieve miniaturized devices for various analytical applications, while featuring low manufacturing costs.^{45,46} However, to prevent background interferences, UV-Vis spectrophotometric techniques necessitate complex sample pre-treatment and call for the employment of various standard chemicals for color transformations.^{43,44} In contrast, an optical chemical sensor promises cheap, reagent-less, and quick experimentation and suffers from less interference during analysis.⁴⁵

Due to the fact that heavy metal ions are harmful to the environment and vital biological processes, there has been a lot of interest in the development of optical sensors for their detection during the past few decades.^{47–53}

Optical sensors are a crucial class of chemical sensors that can track a physical parameter related to a compound's

concentration over time. They offer the benefits of straightforward construction, excellent sensitivity and selectivity, tightly regulated experimental settings, and simple sample processing.^{54,55} Sensors are employed in conjunction with a low-cost spectrophotometric technique to give quick and easy measurement methods with outstanding selectivity and low detection limits.^{23,56}

Reagent immobilization is a crucial step in the fabrication of optical sensors. The immobilization of the sensors' indicators can be accomplished using a variety of chemical and physical techniques. Reagent immobilization is accomplished by physical entrapment,⁵⁷ sol-gel,^{58,59} multilayered films,⁶⁰ or chemical (covalent) bonding methods.⁶¹ Ionophores are crucial components in the design of sensors. As they can form stable complexes with transition metal ions, compounds with different donor atoms are commonly utilized as ionophores in the construction of sensors. For a particular ion, they produce observable sensitivity, selectivity, and stability.⁵⁴

A brief summary of data, including reagents, linear dynamic range, and detection limit of various copper sensors is provided in Table 1. The majority of these copper sensors clearly have one or more of the following drawbacks: a narrow working concentration range, high detection limits, significant cation interference, and irreversible response.

Sensors for the selective detection of Cu²⁺ generally have structures of chelating metal ions with heteroatoms (nitrogen and oxygen/sulfur), such as naphthalimide,^{73,76} naphthalene,⁷⁷ anthracene,⁷⁸ anthraquinone,⁷⁹ quinoline,^{80,81} and macrocyclic^{82,83} derivatives. However, many of them are obtained *via* complex synthesis procedures or require expensive materials. Some Cu²⁺ sensors based on liquid or solid-state membranes have been reported in literature,^{23,65,69,84,85} but they generally have insufficient detection limits, lack sufficient selectivity for environmental sensing, or suffer from reagent leaching problems.

The present work demonstrates the preparation and response of a new highly sensitive copper-optode based on

Table 1 Some optical sensors reported for the determination of Cu²⁺ ions

Reagent	Measured signal	Linear dynamic range (M)	Detection limit (M)	Ref.
Fast sulphon black F	Reflectance	7.9 × 10 ⁻⁵ to 1.6 × 10 ⁻³	2.2 × 10 ⁻⁵	62
Lucifer yellow	Fluorescence	5.0 × 10 ⁻⁸ to 1.0 × 10 ⁻⁴	2.6 × 10 ⁻⁸	63
1-(2-Pyridylazo)-2-naphthol	Absorbance	6.3 × 10 ⁻⁷ to 1.0 × 10 ⁻⁴	3.3 × 10 ⁻⁷	64
(<i>E</i>)- <i>N</i> '-(Pyridin-2-ylmethyl-ene)isonicotin-ohydrazide		1.3 × 10 ⁻⁵ to 8.3 × 10 ⁻⁷	1.9 × 10 ⁻⁷	65
2,2'-Dipyridylamine	Absorbance	7.5 × 10 ⁻⁶ to 2.0 × 10 ⁻⁴	8.0 × 10 ⁻⁷	66
1-(2-Pyridylazo)-2-naphthol	Absorbance	8.0 × 10 ⁻⁶ to 1.3 × 10 ⁻⁴	4.0 × 10 ⁻⁷	67
Zincon	Absorbance	1.6 × 10 ⁻⁶ to 4.7 × 10 ⁻⁵	1.6 × 10 ⁻⁶	68
3-(2-Methyl-2,3-dihydro-1,3-benzothiazol-2-yl)-2 <i>H</i> -chromen-2-one	Absorbance	7.0 × 10 ⁻⁷ to 1.0 × 10 ⁻⁴	3.0 × 10 ⁻⁷	69
L-Cysteine-capped ZnS quantum dots	Fluorescence	0 to 260 × 10 ⁻⁶	7.1 × 10 ⁻⁶	70
DBzDA18C6/PAN	Absorbance	5.0 × 10 ⁻⁷ to 5.0 × 10 ⁻⁵	3.2 × 10 ⁻⁵	71
Pyrocatechol violet	Absorbance	1.0 × 10 ⁻⁵ to 1.0 × 10 ⁻⁴	—	72
6-Bromo-3-(2-methyl-2,3-dihydrobenzo[<i>d</i>]thiazol-2-yl)-2 <i>H</i> -chromen-2-one	Absorbance	7.0 × 10 ⁻⁷ to 1.0 × 10 ⁻⁴	2.5 × 10 ⁻⁷	23
Pyridine-thiourea/PVC	Absorbance	2.0 × 10 ⁻⁴ to 10 × 10 ⁻⁴	1.3 × 10 ⁻⁵	73
Coumarine/triacetylcellulose	Absorbance	8.0 × 10 ⁻⁷ to 1.0 × 10 ⁻⁴	2.5 × 10 ⁻⁷	23
Thiosemicarbazone/triacetylcellulose	Absorbance	7.5 × 10 ⁻⁶ to 2.0 × 10 ⁻⁴	8.0 × 10 ⁻⁸	74
2-(2-Benzothiazolylazo)-3-hydroxyphenol	Absorbance	1.0 × 10 ⁻⁹ to 7.5 × 10 ⁻⁶	3.0 × 10 ⁻¹⁰	This work



covalent immobilization of 2-(2-benzothiazolylazo)-3-hydroxyphenol (BTAHP), which is a Cu^{2+} sensing molecule, on agarose membrane. The low detection limit of the proposed optode allows direct determination of Cu^{2+} in environmental and biological samples without any preconcentration.

Experimental

Reagents

All of the chemicals used were of analytical grade (Merck). Bi-distilled water was used throughout. The stock/standard Cu^{2+} ion solution was prepared by dissolving 0.1278 g of $\text{CuCl}_2 \cdot 2\text{H}_2\text{O}$ in bi-distilled water and diluting it to 250 mL. The solution was standardized *via* titration by a known method.⁸⁶ The method basically depends on the titration of evolving iodine in the presence of starch by the reduction of Cu^{2+} to Cu^+ in the mixtures containing iodide and copper(II) salts. The working standard solutions were prepared by suitable dilution of the stock solution.

Synthesis and purification of the reagent (chemically named 2-(2-benzothiazolylazo)-3-hydroxyphenol) was performed as reported previously.⁸⁷ A solution of 5×10^{-3} M was prepared by dissolving the required weight in ethanol (Merck, Darmstadt, Germany). To hold the agarose membranes within the spectrophotometer quartz cells for absorbance assessments, a homemade polyacrylamide holder was applied. Test samples were buffered in a 0.02 M solution of phosphoric acid/sodium phosphate⁸⁸ and pH was adjusted with dropwise addition of 1.0 M solutions of HCl or NaOH.

Apparatus

The spectroscopic assessments were achieved using a JASCO 530V UV-Vis spectrophotometer. The Cu^{2+} ion detection was evaluated by ICP-AES (PerkinElmer, Germany, 8300). A pH-meter of type Jenway 3505 pH meters 9 V-AC power was employed to record the pH values. The FT-IR spectrum was recorded in KBr pellets on a Shimadzu FT-IR 8101 PC infrared spectrometer in the range of 4000 to 500 cm^{-1} . The thin films were positioned in a quartz cuvette and all absorption investigations were accomplished at 25 ± 2 °C in the batch mode. A homemade polyacrylamide holder was used to hold the agarose membranes inside the quartz cells of the spectrophotometer. A total glass Fisons (UK) double distiller was used to prepare the doubly distilled water.

Procedures

Immobilization procedure. For the preparation of transparent agarose membranes, a method that has been reported elsewhere⁹ was used with some modifications. A weighed amount, *i.e.*, 0.4 g, of agarose powder was mixed with 20 mL of bi-distilled water. To achieve a viscose solution, the mixture was stirred at 90 °C until its volume decreased to 15 mL. The resulting solution was heated at 75 °C until a bubble-free solution was achieved. The final transparent and viscose solution was dispersed between two 20 cm \times 20 cm dust-free glass plates with gentle pressure. The borders of one of the glass

plates were already lined with a 0.25 mm thickness tape to adjust the thickness of the membrane. After cooling, the solidified membrane was cut into appropriate pieces and stored at 4 °C with 50% ethanol solution. For the epoxy activation, an epichlorohydrine method⁸⁹ was used.

For the immobilization of BTAHP on the activated agarose membranes, the membranes were treated with a 5×10^{-3} M BTAHP solution in a sodium phosphate buffer medium with a method reported elsewhere.⁹⁰ The resulting red-colored membranes were thoroughly washed with water on a glass filter, soaked in water overnight, and washed again with a large volume of water to displace any non-bond BTAHP.

Measurement procedure. For spectrophotometric titrations, 2.0 mL of the BTAHP solution (5×10^{-3} M) in water was transferred into a quartz cell of the spectrometer. Microliter volumes of 10^{-4} M solutions of each metal ion were transferred to the BTAHP solution, using a 10 μL Hamilton microsyringe, followed by absorbance readings at 463 nm after vigorous shaking of the cell. All the absorbance data were corrected for the dilution.

A 1 cm \times 2 cm piece of the prepared agarose optode membrane was mounted in a polyacrylamide holder and placed inside the quartz cell of the spectrometer. The absorbance readings were performed against a blank cell containing a non-activated agarose membrane. For the study of the effects of different parameters on the response of the optical membrane, absorbance measurements at 474 nm were performed in an aqueous medium. The calibration curve was accomplished by plotting the absorbance of a series of Cu^{2+} standard solutions at various concentrations. The Cu^{2+} concentration that existed in the sample can be assessed by applying a calibration curve. The optode was regenerated for 5.0 min in a 0.05 M EDTA solution and was then ready to use.

Applications

Analysis of water samples. The proposed sensor was found to work well under laboratory conditions. The Cu^{2+} sensor was used for the determination of Cu^{2+} in some natural water samples. Water samples were collected from a local pipe, river water, and well water (Benha, Egypt). All water samples were filtered through a packed filter to remove particulate impurities, and the pH was adjusted to pH 8.75 by using a buffer solution. This analysis was carried out on 50 mL samples of water following the spiking of the samples with Cu^{2+} ion to make solutions ranging from 65–200 ng mL^{-1} CuCl_2 . The results were compared with those obtained using the ICP-AES method.

Preparation of real foodstuff samples. In order to demonstrate the applicability and reliability of the proposed copper sensor for some real foodstuff samples, black tea, coffee, milk powder, black currant, and sour cherry juice were prepared and analyzed by the suggested method.

Tea and coffee were prepared as follows: the tea or coffee sample (about 1.0 g) was placed in a beaker followed by the addition of 10 mL of HCl and 4.0 mL of HClO_4 . The sample was then digested until the organic residue was completely oxidized. The solution was finally diluted to 100 mL in a standard flask after filtering it through a Whatman filter paper.



The preparation of the black currant and sour cherry juice was performed as follows: the samples were air-dried in porcelain crucibles using an oven at 105 °C for 24 h. Known amounts of dried samples were completely burned in an electric furnace at 500 ± 20 °C. The ashes thus obtained were treated with diluted HCl dissolution.

For analysis of milk samples, about 2.0 g of milk powder was converted to ash at 400 °C in a crucible for 3.0 h. Afterward, 2.0 mL of concentrated HCl was added, and the mixture was heated to dissolve the residue. The pH of the resulting solution was adjusted at optimal value and diluted with bi-distilled water in a 25.0 mL volumetric flask.⁹¹

Analysis of soil sample. The homogenized soil sample (20 g) was weighed accurately; in a 200 mL beaker, it was digested in the presence of an oxidizing agent with the addition of 10 mL of concentrated HNO₃ and 2.0 mL of 70% HClO₄ with heating for 1.0 h. The content of the beaker was filtered through a Whatman no. 40 filter paper into a 250 mL measuring flask; pH was adjusted to the desired value and diluted to mark with bi-distilled water. The general procedure was also applied. Copper levels in the final solutions were determined by ICP-AES using the aforementioned general procedures.

Analysis of vegetable sample. The spinach sample was purchased from Benha, Egypt. Afterward, it was taken in a small mesh. For the digestion of the sample, the procedure described in a previous study⁹² was applied. Forty grams of spinach sample was heated in a silica crucible for 3.0 h on a hot plate, and the charred material was transferred to a furnace for overnight heating at 650 °C. The residue was cooled, and treated with 10 mL of concentrated nitric acid and 3.0 mL 30% H₂O₂; it was again kept in a furnace for 2.0 h at the same temperature so that no organic compound traces were left. The final residue was treated with 3.0 mL of concentrated hydrochloric acid and 2.0–4.0 mL of 70% perchloric acid and evaporated to fumes; the goal was to ensure that all the metals changed to their respective ions. The solid residue was dissolved in water, filtered, and while maintaining the pH at 8.75, the total volume was made up to 25 mL by the addition of buffer solution. The dissolved solution was suitably diluted and the presented procedure was applied.

Analysis of biological samples. Fifty grams of liver or meat were taken and dried for 48 h in an oven at 120 °C to remove the water content and to obtain a constant weight (about 68% of the sample was water). The dried liver or meat sample was transferred into a glass flask. For the digestion of the sample, the procedure given by Ghaedi *et al.*⁹² was applied, and the samples were treated.^{93,94} A concentrated acid mixture of 3.0 mL H₂SO₄, 15 mL of HClO₄, and 15 mL of HNO₃ was added, and the solution was left to stand overnight. The solution was kept in an oil bath at 50 °C until the foaming stopped. The temperature was then increased to 150 °C, and heating was continued until the evolution of the brown fumes of nitrogen oxides ceased. When a dark brown tinge appeared in the mixture, the flask was cooled for about 2.0 min; five milliliters of nitric acid was then added. Heating was continued until the nitrogen oxide fumes were no longer given off. The appearance of white fumes of perchloric acid in 1.0 mL of the solution is an indication of complete digestion. The solid residue

was dissolved in water and filtered; while maintaining the pH at 8.75, the volume was made up to 25 mL by the addition of buffer. The sensor procedure was applied, and the copper levels in the final solutions were determined by ICP-AES and the above-mentioned general procedures.

Accuracy and precision

Six solutions of various concentrations of Cu²⁺ were analyzed to assess the precision and accuracy of the proposed method. Determination of the repeatability (intra-assay) and evaluation of the intermediate precision (inter-assay) were determined over five non-consecutive days; it depended on the relative standard deviation (RSD) percentage that was assessed within the same day, and the six replicates which were evaluated by the assay procedure.

Results and discussion

Preliminary studies

Fig. 1 displays the absorption spectra of BTAHP and the Cu–BTAHP complex solutions, providing valuable insights into their respective maximum absorption wavelengths. Notably, BTAHP exhibits peak absorption at 458 nm, while the Cu–BTAHP complex demonstrates a distinct absorption band at 468 nm. For Cu–BTAHP, the sensor presents an absorbance maximum of ~474 nm. By increasing the addition of Cu²⁺, a decrease in the absorbance is observed at this wavelength. For most of the other metal ions studied, *i.e.*, Mn²⁺, Zn²⁺, Hg²⁺, Cd²⁺, Pb²⁺, Co²⁺, Ni²⁺, Fe²⁺, La³⁺, Fe³⁺, Cr³⁺, Zr⁴⁺, Se⁴⁺, Th⁴⁺, and UO₂²⁺, only negligible or small variations in the absorbance maximum were obtained by altering the metal ion/BTAHP mole ratio. Based on the high selectivity of BTAHP for Cu²⁺ and a distinct color change (decrease) that was observed for the formation of its complex with Cu²⁺, BTAHP was expected to act as a suitable reagent for the preparation of the optode for Cu²⁺ ion (Scheme 1).

Preparation of the optode

For the preparation of the Cu²⁺-sensitive optode, BTAHP was loaded on the transparent agarose membrane. Immobilization


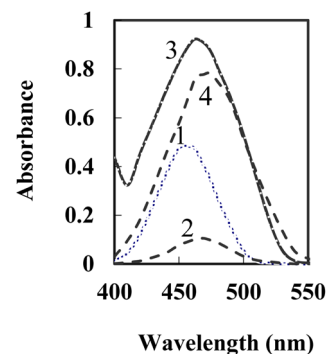


Fig. 1 Absorption spectra of 1-BTAHP in solution; 2-BTAHP–Cu (5×10^{-4} M) in solution and 3-BTAHP optode 4-BTAHP–Cu optode at 5×10^{-7} M Cu²⁺ on the sensor under optimum conditions.



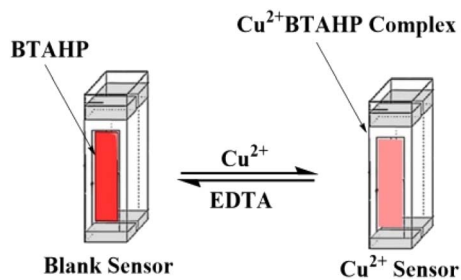

Scheme 1 Representative diagram of the preparation of the Cu^{2+} -sensing optode.

of BTAHP on agarose membranes changed its optical properties to some extent. As depicted in Fig. 1, the absorbance maximum of the BTAHP membrane showed a red shift from 463 to 474 nm, which was probably due to the flatter structure of the immobilized reagent that may have caused an easier electron resonance. Similar shifts have been reported for other agarose optical membranes.^{95–97}

Effect of pH on the test solution

In order to obtain an appropriate BTAHP loading on the agarose membrane, experimental conditions were optimized for immobilization. The effect of pH was studied, which showed that a maximum immobilization of BTAHP was achieved at the pH of ~ 8.75 as recorded in Fig. 2.

A study of the effects of BTAHP concentration on its immobilization on the membrane indicated a continuous increase in the membrane absorbance by an increase in the BTAHP concentration from 2.5×10^{-6} to 5×10^{-2} M. High loadings, however, could unacceptably decrease the transmittance of the membrane. Therefore, a BTAHP concentration of 5×10^{-3} M, resulting in a maximum absorbance of about 0.73, was used in subsequent experiments.

BTAHP contains an azo group, and it shows color changes with pH variation as reported elsewhere.⁸⁷ Therefore, the response characteristics of the membrane prepared for Cu^{2+} determination were studied as a function of pH. It seemed more

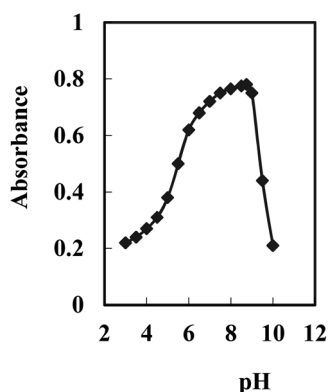


Fig. 2 Effect of pH on the optode of 5×10^{-7} M Cu^{2+} complexed with BTAHP under optimum conditions.

appropriate to use ΔA (the difference in absorbance before and after the addition of Cu^{2+}) rather than the absolute value of A in this investigation. The difference in absorbance increased rapidly from 4.5 to 7.5, then slightly increased till it became pH 8.75; it started to decrease from \sim pH 9.0 and decreased rapidly at higher pH values. Therefore, a pH of 8.75 was considered to be optimum and was used for the determination of Cu^{2+} in test solutions.

Effect of temperature on the sensor reaction

The effect of temperature on the performance of the sensor was studied. The absorption spectra were recorded at various temperatures 25 to 70 °C at 474 nm. As the temperature of the Cu^{2+} sample increased, the difference in absorbance at 474 nm decreased due to thermal quenching, which was related to the increase in ions lattice vibrations⁹⁸ and decreasing formation of the complex with the membrane. Increasing the temperature to ≥ 75 °C eliminated the variation in absorbance indicating no complex formation between Cu^{2+} and BTAHP. The best temperature to obtain highly sensitive and selective results was 25 ± 2.0 °C.

Response time of the optode

The response time of the Cu^{2+} optode membrane was evaluated by immersing the optode in a 5×10^{-7} M Cu^{2+} solution, buffering it at pH 8.75, and following the absorbance change at 474 nm with time. As shown in Fig. 3, the absorbance reached 95% of the steady-state signal in ~ 3.0 min.

Generally, the response time decreased by increasing the analyte concentration and varying it from 2.0 to 3.0 min. This may be explained by the fact that at higher analyte concentrations, the rate of diffusion of the analyte in the membrane phase may be increased.⁹⁹

Stoichiometric ratio

The binding mode of BTAHP with Cu^{2+} was confirmed by the absorbance of the Job plot method. To obtain the Job plot, the experiment was performed between BTAHP and different moles ratio of Cu^{2+} ions; the maximum difference in absorbance was observed at 0.5 mole fraction of the sensor, which indicated 1 : 1

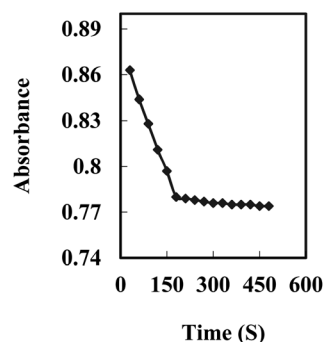


Fig. 3 A typical response curve of the optode at 474 nm as a function of time for Cu^{2+} concentration of 5×10^{-7} M.



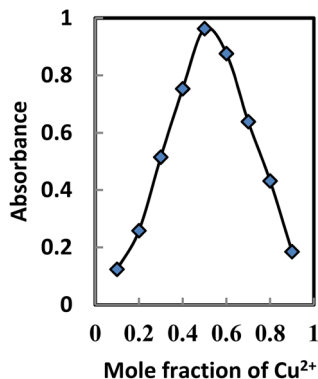


Fig. 4 Job's method for the determination of the Cu^{2+} -BTAHP complex.

stoichiometric complexation (Fig. 4). These findings, combined with the infrared (IR) spectra of BTAHP and the Cu -BTAHP complex, provided the basis for proposing a structural representation of the complex as depicted in Scheme 2. The Cu ion formed a covalent bond with the oxygen atom of the hydroxyl group and a coordinate bond with the nitrogen atom of the azo group. For the 1 : 1 binding mode, the conditional formation constant ($\log K$), was evaluated using the Harvey and Manning equation by applying the data obtained from the Job's method; the result was a value of 8.57, whereas the true constant was 8.70. The mechanism of formation of the optode membrane and complex is represented in Scheme 2.

Regeneration, reproducibility, short-term stability, and lifetime

Efficient regeneration of the sensor in a reasonable time is a requirement for its usefulness in multiple usages. HCl , NaSCN , and EDTA solutions were tested in different concentrations for the possible regeneration of the membrane after it had been loaded by Cu^{2+} samples to be examined. The results indicated that a 0.05 M EDTA solution can efficiently remove

any adsorbed Cu^{2+} from the membrane and return its absorbance to the initial value in ~ 5.0 min (Fig. 5).

The reproducibility of the membrane optode response was investigated by its multiple usages for Cu^{2+} monitoring in test solutions of 5×10^{-7} M. After each absorbance reading, the membrane was regenerated by a 0.05 M EDTA solution, rinsed with some deionized water, and soaked in a phosphate buffer solution (pH 8.75) for a few minutes. Good reproducibility was obtained for the signal at a Cu^{2+} concentration of 5×10^{-7} M. The corresponding RSD value was found to be $\pm 1.9\%$.

The results of the intra-day and inter-day precision and accuracy assessments indicated that the approach applied here was highly repeatable and reproducible; the coefficients of variation ranged between 1.65 and 1.90%.

The short-term stability of the proposed sensor was studied by variation in the absorbance measurements, when the sensor was in contact with a 5×10^{-7} M Cu^{2+} solution at pH 8.75 over a period of 5.0 h. From the absorbance value that was taken every 10 min ($n = 30$), it was found that the response was almost complete with only a 2.7% increase in absorbance after 5.0 h of monitoring.


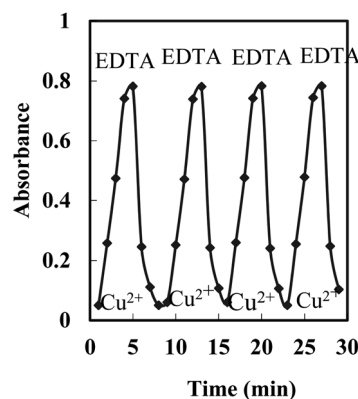


Fig. 5 Repeatability of the optode exposed to 100 ng mL^{-1} of Cu^{2+} and 0.05 M EDTA .



Scheme 2 Representative scheme of the optode and BTAHP-Cu^{2+} complex formation.

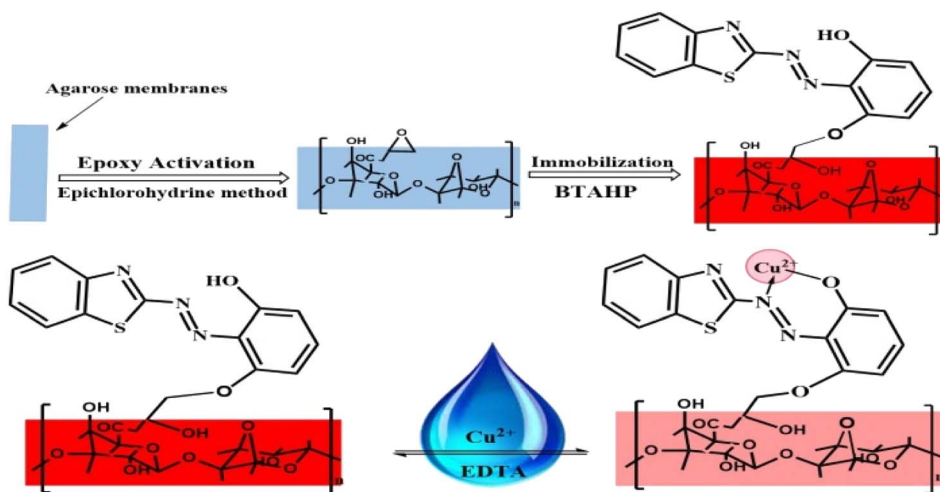

The lifetime of the membrane was examined over a period of two months during which four prepared membranes were stored in 20% ethanol at 4 °C. The mean absorbance differences of the sensors at 474 nm were found to be 0.057 (± 0.0015) and 0.058 (± 0.0019) before and after this period, respectively. Hence, the sensor is stable within this period with a minimum lifetime of two months. In addition, no evidence of dye leaching or signal drift was observed during multiple usages of the membrane.

Effect of interfering ions

For the selectivity investigation, the interference of different inorganic cations on the response of the proposed sensor was tested using solutions of 5×10^{-7} M of Cu^{2+} and variable concentrations of interfering cations in phosphate buffer (pH 8.75). The tolerance limit was considered to be the concentration that caused an error of more than $\pm 5.0\%$ in the absorbance difference corresponding to a fixed concentration of Cu^{2+} ions. Based on the data shown in Table 2, it can be seen that BTAHP-based optode is highly selective towards the Cu^{2+} ion, and it tolerates 400 times or higher concentrations of monovalent, divalent, trivalent, and tetravalent diverse ions. The results confirmed that the optode exhibited excellent selectivity toward Cu^{2+} ions with respect to the other coexisting interference ions at $\lambda_{\text{max}} = 474$ nm. Although zirconium formed a complex with BTAHP at a pH of 5.5 on a dextran-type lipophilic gel and was measured at 569 and 800 nm by applying solid-phase spectrophotometry, it does not react under conditions that are optimized for the proposed optode for Cu ion.

Calibration curve

The membrane response curve was studied by the stepwise addition of Cu^{2+} to a series of test solutions, followed by monitoring the differences in absorbance at 474 nm. It was found that the absorbance decreased continuously by increasing the analyte concentration, and the membrane was saturated when the Cu^{2+} concentration exceeded 7.5×10^{-7} M. The response curve was linear in a logarithmic scale for a Cu^{2+} concentration range of 7.5

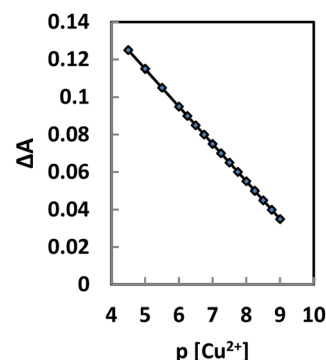


Fig. 6 Logarithmic scale calibration curve for the Cu^{2+} optode at 474 nm under optimum conditions.

$\times 10^{-6}$ to 1.0×10^{-9} M (Fig. 6). A line was fitted to the experimental points, and the following equation was achieved for the calibration curve with an R^2 value of 0.9988:

$$\Delta A = -0.0206\text{pCu} + 0.2184 \quad (1)$$

Here, pCu stands for $-\log[\text{Cu}^{2+}]$. The detection and quantification limits were evaluated by ordinary methods from 3σ and 10σ to be 3.0×10^{-10} and 9.8×10^{-10} M, respectively, which is sufficiently low for the detection of Cu^{2+} in environmental samples.

The performance of the proposed sensor was assessed by evaluation of the t -value (for accuracy) and F -test (for precision) as compared with the ICP-AES method. The mean values were obtained in a Student's t - and F -tests at 95% confidence limits for five degrees of freedom.¹⁰⁰ The results showed that the calculated values did not exceed the theoretical values. The wider range of determination, higher accuracy, increased stability, and lower time consumption shows the advantages of the proposed method over the compared method.

Accuracy and precision

To check the validity, accuracy, and applicability of the proposed method and the reproducibility of the results

Table 2 Effect of the possible interferences on the absorbance of the optode

Interferent	Concentration (M)	Absorbance change ($\Delta A = A_2 - A_1$)	Relative error ($\Delta A/A_1 \times 100$)
K^+ , Na^+	2×10^{-4}	0.015	1.92
Ag^+ , Li^+	2×10^{-4}	0.023	2.94
Ca^{2+} , Mg^{2+}	2×10^{-4}	0.18	2.30
Mn^{2+} , Zn^{2+}	2×10^{-4}	0.027	3.95
Pb^{2+} , Hg^{2+}	2×10^{-4}	0.031	3.96
Co^{2+} , Ni^{2+}	2×10^{-4}	0.033	4.22
Cd^{2+} , Fe^{2+}	2×10^{-4}	0.35	4.48
Fe^{3+} , Al^{3+}	2×10^{-4}	0.034	4.35
La^{3+} , Cr^{3+}	2×10^{-4}	0.32	4.09
Y^{3+} , Sm^{3+}	2×10^{-4}	0.30	3.84
Zr^{4+} , Se^{4+}	2×10^{-4}	0.39	4.84
Th^{4+} , UO_2^{2+}	2×10^{-4}	0.36	4.69



presented, six replicate experiments at six concentrations of Cu^{2+} ions were carried out. The relative standard deviations of the various Cu^{2+} concentrations that were obtained from the experiments were carried out. It was found that the within-day relative standard deviations were <1.7%, indicating that the proposed method was highly reproducible and that BTAHP was successfully applied to determine Cu^{2+} in the complex formation.

Performance comparison of the Cu^{2+} ion optode with other works

There are several Cu^{2+} ion detection methods reported in the literature based on reflectance,⁶² fluorescence,^{63,70} transducers, optical absorption,^{23,64–69,71–74} and the use of different immobilization substrates. A comparison of the sensing performance of the Cu^{2+} ion optode developed in this work with similar methods from other literature reports is summarized in Table 1 with regard to dynamic linear response range and limit of detection. The developed Cu^{2+} ion optode was noted to exhibit improved dynamic linear range with shorter response time, *i.e.*, within 3.0 min as compared to other reported optical Cu^{2+} ion optodes. This was largely due to the large surface area of BTAHP that provided multiple binding sites for immobilization of the chemical sensing reagent, which considerably increased the diffusion rate of the target analyte and the loading capacity of both the reactant and the target. Moreover, the utilization of a BTAHP multi-dentate derivative as the sensing reagent also promoted higher binding capacity due to the availability of

multi-banding sites of the BTAHP reagent for Cu^{2+} ions. The use of agarose as the immobilization matrix, on the other hand, was reported to be beneficial for a wider working linear range in the quantification of Cu^{2+} ions.⁴⁴ The proposed optode, which was based on immobilized BTAHP as an ionophore, for Cu^{2+} ion detection demonstrated no leaching of the sensing materials from the micro-sized immobilization substrate due to the excellent compatibility between the lipophilic BTAHP ligand compound.

Analytical performance

Determination of copper ions in drinking water samples.

Copper is an essential trace element required to maintain good health as it plays a vital role in several enzymes. A normal adult requires 2–4 mg of copper per day most of which is provided by food and ~10% comes from drinking water. However, consumption of excessive levels of copper can cause nausea, vomiting, diarrhea, and headaches. The USEPA (United States Environmental Protection Agency) and European Council Directive proposed the Maximum Contaminant Level for Cu in drinking water to be $1.3 \mu\text{g mL}^{-1}$.¹⁰¹ It is necessary to make an accurate, fast, and cheap optode for the determination of Cu(II) in water.

Analysis of the spiked copper samples further proved the validity of the proposed procedure. For this reason, the solutions of concentrations between 1.0 and $3.0 \mu\text{g mL}^{-1}$ were spiked in the sample by using 50 mL of a water sample. Copper was assessed using the proposed optode after the samples were

Table 3 Recovery studies of copper in real samples

Sample	Added ng mL^{-1}	Found ^a ng mL^{-1}		RSD (%)	Recovery (%)	<i>t</i> -Test ^b	<i>F</i> -Value ^b
		Sensor	ICP-AES				
Tap water	0.0	6.6	6.3	—	—	—	—
	100	106.0	106.5	1.7	99.44	—	3.84
	200	209.5	203.1	1.5	101.40	1.59	—
Well water	0.0	77.0	75.5	—	—	—	—
	70	149.0	142.3	1.2	101.36	—	3.32
	140	213.2	218.7	1.4	98.25	1.42	—
River water	0.0	61.5	63.0	—	—	—	—
	65	123.8	125.0	1.6	97.87	—	3.57
	130	195.8	197.8	1.4	102.25	1.08	—
Vegetable	0.0	28.5	28.8	—	—	—	—
	50	79.0	76.8	1.3	100.64	—	3.41
	100	127.0	131.5	1.6	98.83	1.72	—
Lotus (tree)	0.0	18.0	17.8	—	—	—	—
	90	107.0	110.6	1.1	99.07	—	3.68
	180	200.0	194.3	1.5	99.13	1.25	—
Liver	0.0	29.5	29.0	—	—	—	—
	75	106.0	111.7	1.1	101.44	1.81	—
	150	178.0	185.3	1.4	99.16	—	3.52
Meat	0.0	31.0	30.5	—	—	—	—
	60	90.4	88.8	1.7	99.34	1.66	—
	120	152.5	154.7	1.5	100.99	—	3.28
Soil	0.0	17.6	18.1	—	—	—	—
	80	99.0	95.6	1.4	101.43	1.53	—
	160	178.4	180.9	1.2	100.45	—	2.92

^a Average of six replicate measurements. ^b Theoretical values of *t* and *F* at 95% confidence limit were 2.57 and 5.05, respectively.



homogenized, and the proposed methodology was implemented. Analytical parameters derived from standard studies as provided for the proposed method were used to derive the

results. Table 3 showed the experimental results of spiked copper samples. The RSDs were below 2.15%. Calculated recoveries for waters were found between 98.33 and 102.67%.

Table 4 Results obtained by the application of the proposed Cu²⁺ sensor to some foodstuff products

Sample	Added $\mu\text{g g}^{-1}$	Found ^a $\mu\text{g g}^{-1}$		Recovery (%)	<i>t</i> -Test ^b	<i>F</i> -Value ^b
		Proposed	ICP-AES			
Coffee	—	1.86 ± 0.31	1.91 ± 0.56	—		
	2.5	4.45 ± 0.38	4.20 ± 0.82	102.06	1.09	
	5.0	6.75 ± 0.24	7.00 ± 0.63	98.40		3.77
	7.5	9.55 ± 0.17	9.15 ± 0.90	102.27	1.37	
Black tea	—	4.39 ± 0.32	4.47 ± 0.77	—		
	5.0	9.20 ± 0.42	9.70 ± 0.95	97.98		3.57
	10	14.55 ± 0.23	14.15 ± 0.86	101.11	1.43	
Black currant	—	20.00 ± 0.37	19.00 ± 0.67	103.15		3.87
	7.5	4.97 ± 0.21	5.11 ± 0.84	—		
	15	12.55 ± 0.24	12.80 ± 0.97	100.64	1.47	
Sour cherry juice	—	19.70 ± 0.19	20.40 ± 0.81	98.65		3.16
	7.5	27.25 ± 0.45	27.85 ± 0.78	99.20	1.56	
	22.5	0.61 ± 0.25	0.69 ± 1.04	—		
Milk powder	—	2.15 ± 0.29	2.00 ± 0.79	101.90		3.68
	1.5	3.70 ± 0.18	3.40 ± 1.03	102.49	1.32	
	3.0	5.00 ± 0.39	5.35 ± 0.88	97.85		3.17
Milk powder	—	4.20 ± 0.33	4.15 ± 0.69	—		
	3.0	7.15 ± 0.28	7.35 ± 0.85	99.31	1.17	
	6.0	10.45 ± 0.41	9.90 ± 1.01	102.45		3.68
	9.0	13.00 ± 0.34	13.45 ± 1.07	98.48	1.46	

^a Average of six replicate measurements ± standard deviation. ^b Theoretical values of *t* and *F* at 95% confidence limit were 2.57 and 5.05, respectively.

Table 5 Results obtained for Cu(II) determination in six edible oil samples

Sample	Spiked ng L^{-1}	Found ^a (ng L^{-1}) ± SD		Recovery, %	<i>t</i> -Test ^b	<i>F</i> -Value ^b
		Proposed	FAAS			
Extra virgin olive oil	—	75.0 ± 0.44	75.5 ± 1.21	—	—	
	250	281.5 ± 0.27	267.5 ± 1.43	102.36	1.65	
	500	564.5 ± 0.18	588.0 ± 1.73	98.17		3.28
	750	842.0 ± 0.29	811.5 ± 1.50	102.60	1.23	
Soybean oil	—	76.0 ± 0.16	75.35 ± 1.27	—		
	300	368.5 ± 0.21	392.0 ± 1.62	98.01	1.72	
	600	694.0 ± 0.26	662.0 ± 1.38	102.66		3.18
Chilli oil	—	1000 ± 0.19	954.5 ± 1.15	102.46	1.34	
	200	109.0 ± 0.13	108.50 ± 1.52	—		
	400	303.5 ± 0.31	315.0 ± 1.37	98.22	1.17	
Palm oil	—	515.5 ± 0.25	500.0 ± 1.53	102.38		3.44
	600	720.0 ± 0.21	695.5 ± 1.31	101.55	1.86	
	1050	99.0 ± 0.15	100.50 ± 0.88	—		
Rice bran oil	—	458.5 ± 0.27	466.5 ± 0.96	102.12		2.84
	350	792.0 ± 0.33	715.0 ± 1.56	99.12	1.55	
	700	1135.5 ± 0.37	1125.0 ± 1.44	98.78		3.63
Corn oil	—	91.0 ± 0.18	91.5 ± 1.76	—		
	400	482.5 ± 0.31	500.5 ± 1.21	98.27	1.79	
	800	909.0 ± 0.34	873.5 ± 1.17	102.02		3.52
Corn oil	—	1307 ± 0.22	1266.0 ± 0.95	101.24	1.48	
	500	77.5 ± 0.29	77.0 ± 1.32	—		
	1000	565.0 ± 0.12	593.5 ± 1.04	97.84		3.83
	1500	1100 ± 0.51	1105.0 ± 1.72	102.09	1.81	
	1500	1559.5 ± 0.38	1600.0 ± 1.47	98.86		3.69

^a Average of six replicate measurements ± standard deviation. ^b Theoretical values of *t* and *F* at 95% confidence limit are 2.57 and 5.05, respectively.



Determination of copper ions in environmental samples. In order to confirm the applicability of the proposed sensor procedure, it has been used to determine nanogram amounts of Cu^{2+} in environmental (vegetable biological and soil) samples. The reliability of the presented procedure was checked by spiking experiments and independent analysis. The results are presented in Table 3. An ICP-AES methodology was applied as the reference method, and the results are shown in Table 3. The recovery of spiked samples is satisfactorily reasonable and was confirmed using the standard addition method, which indicates the capability of the system to determine the ions. A good agreement was achieved between the added and measured analyte amounts. The recovery values evaluated for the added standards were always higher than 95%, thus confirming the accuracy of the method and its independence from the matrix effects.

Determination of copper ions in foodstuff samples. The proposed sensor was considered to be an ideal choice for the target analyte determination in a wide variety of real foodstuff samples as they possess numerous advantages, such as simplicity, speed, low cost, possibility of rapid sampling, and selectivity.

To assess the applicability of the proposed Cu^{2+} sensor, an attempt was made to determine the Cu^{2+} ion concentration in some real foodstuff samples. The samples were treated by the reported procedures as described above and analyzed by the proposed sensor. The analysis was performed by the standard addition technique. The results are presented in Table 4. According to this Table 4, the obtained results are comparable with those obtained by ICP-AES. Thus, the optode is a good alternative method for the determination of Cu^{2+} in different real samples.

The performance of the optode was assessed by calculation of the t -value (for accuracy) and F -test (for precision) as compared with the ICP-AES method. The mean values were obtained in a Student's t - and F -tests at 95% confidence limits for five degrees of freedom.¹⁰⁰ The results showed that the calculated values did not exceed the theoretical values indicating no significant difference with the compared procedure.

The data (Table 5) reveal a reasonable consistency within the assessed values through the proposed technique for six edible oil samples and that conventionally depend on ICP-AES for Cu quantitation. Accuracy was assessed by comparing results with those from the ICP-AES. Applying the paired t -test and F -value shows no significant differences at a 95% confidence level.

Conclusion

The BTAHP-based Cu^{2+} optode membrane developed in this study exhibits excellent Cu^{2+} selectivity as compared to other common metal ions. For direct evaluation of the analyte in samples of polluted natural water, the optode exhibits great sensitivity and low detection and quantification limits. Simple membrane preparation and the development of a covalent bond between BTAHP and the agarose membrane help form an optode with a long lifetime and a rapid reaction time that does not show any signs of dye leaching. The optode membrane may

be easily regenerated by an EDTA solution; it also offers the possibility of multiple usages for environmental monitoring of Cu^{2+} . Due to the advantages of the proposed optode method with respect to previously reported ones (Table 1), it may be used as a promising alternative for copper determination in water, food, and environmental samples.

Data availability

All data and materials will be made available upon request.

Author contributions

Mai Aish: conceptualization, data curation, investigation, methodology, validation, visualization, writing – original draft, writing – review & editing. Validation, writing – original draft, writing–review & editing. Reem Alshehri: conceptualization, investigation, methodology, validation, writing – original draft, writing – review & editing. Alaa Amin: conceptualization, methodology, data curation, investigation, supervision, writing–original draft, writing – review & editing.

Conflicts of interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported.

Acknowledgements

The authors offer their sincere thanks to Port Said, Taibah, and Benha Universities for providing the necessary facilities.

References

- 1 G. Forstner and T. Wittmann, *Metal pollution in the aquatic environment*, Springer Verlag, Newyork, 1981, vol. 3, pp. 271–318.
- 2 Q. Meng, R. Zhang, H. Jia, X. Gao, C. Wang, Y. Shi, *et al.*, *Talanta*, 2015, **143**, 294–301.
- 3 F. Bulcke, R. Dringen and I. F. Scheiber, Neurotoxicity of Copper. *Neurotoxicity of Metals*. Springer, 2017, pp. 313–343.
- 4 I. F. Scheiber, J. F. Mercer and R. Dringen, *Prog. Neurobiol.*, 2014, **116**, 33–57.
- 5 B. E. Kim, T. Nevitt and D. J. Thiele, *Nat. Chem. Biol.*, 2008, **4**, 176–185.
- 6 J. Prohaska and A. A. Gybina, *J. Nutr.*, 2004, **134**, 1003–1006.
- 7 E. Que, D. W. Domaille and C. J. Chang, *Chem. Rev.*, 2008, **108**, 1517–1549.
- 8 A. V. Davis and T. V. O'Halloran, *Nat. Chem. Biol.*, 2008, **4**, 148–151.
- 9 N. J. Robinson and D. R. Winge, *Annu. Rev. Biochem.*, 2010, **79**, 537–562.
- 10 E. Gaggelli, H. Kozłowski, D. Valensin and G. Valensin, *Chem. Rev.*, 2006, **106**, 1995–2044.
- 11 I. Bertini and A. Rosato, *Cell. Mol. Life Sci.*, 2008, **65**, 89–91.
- 12 S. G. Kaler, *Nat. Rev. Neurol.*, 2011, **7**, 15–29.



- 13 A. Ahuja, K. Dev, R. S. Tanwar, K. K. Selwal and P. K. Tyagi, *J. Trace Elem. Med. Biol.*, 2015, **29**, 11–23.
- 14 P. Dusek, P. M. Roos, T. Litwin, S. A. Schneider, T. P. Flaten and J. Aaseth, *J. Trace Elem. Med. Biol.*, 2015, **31**, 193–203.
- 15 Y. H. Hung, A. I. Bush and R. A. Cherny, *J. Biol. Inorg. Chem.*, 2010, **15**, 61–76.
- 16 H. Kozłowski, M. Luczkowski, M. Remelli and D. Valensin, *J. Biol. Inorg. Chem.*, 2012, **256**, 2129–2141.
- 17 R. Squitti, I. Simonelli, E. Cassetta, D. Lupoi, M. Rongioletti, M. Ventriglia and M. Siotto, *Curr. Alzheimer Res.*, 2017, **14**, 1318–1326.
- 18 D. Strausak, J. F. Mercer, H. H. Dieter, W. Stremmel and G. Multhaup, *Brain Res. Bull.*, 2001, **55**, 175–185.
- 19 G. Multhaup, A. Schlicksupp, L. Hesse, D. Beher, T. Ruppert, C. L. Masters and K. Beyreuther, *Science*, 1996, **271**, 1406–1409.
- 20 I. Yreula, *Braz. J. Plant Physiol.*, 2005, **17**, 145–156.
- 21 M. Kumar and A. Puri, A review of permissible limits of drinking water, *Indian J. Occup. Health*, 2012, **16**, 40–44.
- 22 J. J. Pinto, C. Moreno and M. Garcia-Vargas, *Talanta*, 2004, **64**, 562–565.
- 23 E. Pourbasheer, S. Morsalia, A. Banaei, S. Aghabalazadeh, M. R. Ganjali and P. Norouzi, *J. Ind. Eng. Chem.*, 2015, **26**, 370–374.
- 24 C. Boonmee, T. Noipa, T. Tuntulani and W. Ngeontae, *Spectrochim. Acta, Part A*, 2016, **169**, 161–168.
- 25 M. Camino, M. G. Bagur and M. Sa, *J. Anal. At. Spectrom.*, 2001, **16**, 638–642.
- 26 R. J. Cassella, O. I. B. Magalh, M. Tadeu, E. Luiz, S. Lima, M. Ang, F. S. Neves, F. Margarida and B. Coutinho, *Talanta*, 2005, **67**, 121–128.
- 27 B. F. Reis, M. Knochen, G. Pignalosa, N. Cabrera and J. Giglio, *Talanta*, 2004, **64**, 1220–1225.
- 28 M. H. Mashhadizadeh, M. Pesteh, M. Talakesh, I. Sheikhshoae, M. M. Ardakani and M. A. Karimi, *Spectrochim. Acta, Part B*, 2008, **63**, 885–888.
- 29 K. Pomazal, C. Prohaska, I. Steffan, G. Reich and F. K. Josef, *Analyst*, 1999, **124**, 657–663.
- 30 L. C. Ferreira, A. S. Queiroz, M. S. Fernandes and H. C. Santos, *Spectrochim. Acta, Part B*, 2002, **57**, 1939–1950.
- 31 A. Asfaw and G. Wibetoe, *Microchim. Acta*, 2005, **68**, 61–68.
- 32 A. A. Vaughan and R. Narayanaswamy, *Sens. Actuators, B*, 1998, **51**, 368–376.
- 33 J. S. Becker, A. Matusch, C. Depboylu, J. Dobrowolska and M. V. Zoriy, *Anal. Chem.*, 2007, **79**, 6047–6080.
- 34 D. Walaszek, M. Senn, A. Wichser, M. Faller, B. Wagner, E. Bulska and A. Ulrich, *Spectrochim. Acta, Part B*, 2014, **99**, 115–120.
- 35 B. Yin, Z. Liu, M. Yi and J. Zhang, *Tetrahedron Lett.*, 2008, **49**, 3687–3690.
- 36 A. P. S. Gonzales, M. A. Firmino, C. S. Nomura, F. R. P. Rocha, P. V. Oliveira and I. Gaubeur, *Anal. Chim. Acta*, 2009, **636**, 198–204.
- 37 A. Mohadesi and M. A. Taher, *Talanta*, 2007, **72**, 95–100.
- 38 A. A. Ensafi, T. Khayamian, A. Benvidi and E. Mirmomtaz, *Anal. Chim. Acta*, 2006, **561**, 225–232.
- 39 C. Topcu, G. Lacin, V. Yilmaz, F. Coldur, B. Caglar and I. Isildak, *Anal. Lett.*, 2018, **51**, 1890–1910.
- 40 M. A. Chamjangali, S. Soltanpanah and N. Goudarzi, *Sens. Actuators, B*, 2009, **138**, 251–256.
- 41 X. Zhang, J. Peng, C. He, G. Shen and R. Yu, *Anal. Chim. Acta*, 2006, **567**, 189–195.
- 42 T. Mayr and T. Werner, *Analyst*, 2002, **127**, 248–252.
- 43 L. L. Tan, A. Musa and Y. H. Lee, *Sens. Actuators, B*, 2012, **173**, 614–619.
- 44 S. S. M. Hassan, S. A. Marei, I. H. Badr and H. A. Arida, *Anal. Chim. Acta*, 2001, **427**, 21–28.
- 45 H. Filik and D. Aksu, *Sens. Actuators, B*, 2009, **136**, 105–112.
- 46 P. L. Yew and Y. H. Lee, *Sens. Actuators, B*, 2014, **191**, 719–726.
- 47 A. Tigrerosa and J. Portilla, *RSC Adv.*, 2020, **10**, 19693–19712.
- 48 P. Grandjean, P. Weihe, R. F. White and F. Debes, *Environ. Res.*, 1998, **77**, 165–172.
- 49 B. High, D. Bruce and M. M. Richter, *Anal. Chim. Acta*, 2001, **449**, 17–22.
- 50 L. Tapia, M. Suazo, C. Hodar, V. Cambiazo and M. Gonzalez, *BioMetals*, 2003, **16**, 169–174.
- 51 D. J. Waggoner, T. B. Bartnikas and J. D. Gitlin, *Neurobiol. Dis.*, 1999, **6**, 221–230.
- 52 H. Jiang, D. Tang, Z. Li, J. Li, H. Liu, Q. Meng, Q. Han and X. Liu, *Spectrochim. Acta, Part A*, 2020, **243**, 118784.
- 53 H. B. Wang, H. Y. Bai, Y. S. Wang, T. Gan and Y. M. Liu, *Microchim. Acta*, 2020, **187**, 185–189.
- 54 R. Zare-Dorabei, K. Dashtian and V. Jalalat, *IEEE Sens. J.*, 2015, **15**, 6715–6718.
- 55 R. Zare-Dorabei, P. Norouzi and M. R. Ganjali, *J. Hazard. Mater.*, 2009, **171**, 601.
- 56 K. Alizadeh, B. Rezaei and E. Khazaeli, *Sens. Actuators, B*, 2014, **193**, 267–271.
- 57 H. Xu, J. W. Aylott, R. Kopelman, T. J. Miller and M. A. Philbert, *Anal. Chem.*, 2001, **73**, 4124.
- 58 S. Dong, M. Luo, G. Peng and W. Cheng, *Sens. Actuators, B*, 2008, **129**, 94–98.
- 59 K. Dashtian and R. Zare-Dorabei, *Sens. Actuators, B*, 2017, **242**, 586–590.
- 60 M. Swati, N. Nisha and R. Srivastava, *J. Bionanosci.*, 2007, **1**, 90–96.
- 61 R. Güell, C. Fontàs, V. Salvadó and E. Anticó, *Anal. Chim. Acta*, 2007, **594**, 162–167.
- 62 W. E. F. W. Khalid, M. Ahmad and L. Y. Heng, *Chiang Mai J. Sci.*, 2014, **41**, 383–389.
- 63 N. Aksuner, E. Henden, I. Yilmaz and A. Cukurovali, *Sens. Actuators, B*, 2008, **134**, 510.
- 64 B. Rezaei, H. Hadadzadeh and A. Azimi, *J. Anal. Chem.*, 2012, **67**, 687–691.
- 65 M. Ghaedi, A. Shahamiri, S. Hajati and B. Mirtamizdoust, *J. Mol. Liq.*, 2014, **199**, 483–488.
- 66 R. Zare-Dorabei, S. M. Ferdowsi, A. Barzinand and A. Tadjarodi, *Ultrason. Sonochem.*, 2016, **32**, 265–276.
- 67 M. Ghaedi, J. Tashkhourian, M. Montazerzohori, M. N. Biyareh and B. Sadeghian, *Arabian J. Chem.*, 2017, **10**, S2319.



- 68 T. Leelasattarakul, S. Liawruangrath, M. Rayanakorn, B. Liawruangrath, W. Oungpipat and N. Youngvises, *Talanta*, 2007, **72**, 126–131.
- 69 E. Pourbasheer, S. Morsali, Z. Azari, M. A. Karimi and M. R. Ganjali, *Appl. Organomet. Chem.*, 2018, **32**, 1–8.
- 70 M. Koneswaran and R. Narayanaswamy, *Sens. Actuators, B*, 2009, **139**, 104–108.
- 71 N. Alizadeh, A. Moemeni and M. Shamsipur, *Anal. Chim. Acta*, 2002, **464**, 187–191.
- 72 I. M. Steinberg, A. Lobnik and O. S. Wolfbeis, *Sens. Actuators, B*, 2003, **90**, 230–235.
- 73 W. M. Khairul, M. F. Abu Hassan, A. I. Daud, H. M. Zuki, K. H. K. Bulat and M. A. Kadir, *Malaysian J. Anal. Sci.*, 2016, **20**, 73–84.
- 74 M. A. Chamjangali, S. Soltanpanah and N. Goudarzi, *Sens. Actuators, B*, 2009, **138**, 251–256.
- 75 H. Cheng and Y. Qian, *Dyes Pigm.*, 2015, **112**, 317–326.
- 76 M. Dodangeh, K. Gharanjig and M. Arami, *Spectrochim. Acta, Part A*, 2016, **154**, 207–214.
- 77 J. Dessingiou, J. K. Khedkar and C. P. Rao, *J. Chem. Sci.*, 2014, **126**, 1135–1141.
- 78 H. G. Lee, K. B. Kim, G. J. Park, Y. J. Na, H. Y. Jo, S. A. Lee and C. Kim, *Inorg. Chem. Commun.*, 2014, **39**, 61–65.
- 79 K. Ghosh and D. Kar, *J. Inclusion Phenom. Macrocyclic Chem.*, 2013, **77**, 67–74.
- 80 L. Tang, P. Zhou, Z. Huang, J. Zhao and M. Cai, *Bull. Korean Chem. Soc.*, 2013, **34**, 2905–2908.
- 81 J. Jiang, H. Jiang, X. Tang, L. Yang, W. Dou, W. Liu, R. Fang and W. Liu, *Dalton Trans.*, 2011, **40**, 6367–6370.
- 82 P. N. Basa and A. G. Sykes, *J. Org. Chem.*, 2012, **77**, 8428–8434.
- 83 P. Singh, L. S. Mittal, S. Kumar, G. Bhargava and S. Kumar, *J. Fluoresc.*, 2014, **24**, 909–915.
- 84 N. H. Abdul Razak, L. L. Tan, S. A. Hasbullah and L. Y. Heng, *Microchem. J.*, 2020, **153**, 104460.
- 85 L. K. Kumawata, N. Mergua, A. K. Singh and V. K. Gupta, *Sens. Actuators, B*, 2015, **212**, 389–394.
- 86 A. I. Vogel, *A Text-Book of Quantitative Inorganic Analysis*, 3rd edn, Longmans, London, 1961, p. 441.
- 87 A. S. Amin, *J. Taibah Univ. Sci.*, 2015, **9**, 227–236.
- 88 J. A. Dean, *Analytical Chemistry Handbook*, McGraw-Hill, New York, 1995, pp. 14.30–14.34.
- 89 I. Matsumoto, Y. Mizuno and N. Seno, *J. Biochem.*, 1979, **85**, 1091–1096.
- 90 P. Hashemi and M. M. Abolghasemi, *Sens. Actuators, B*, 2006, **115**, 49–53.
- 91 A. K. Singh, S. Mehtaband and A. K. Jain, *Anal. Chim. Acta*, 2006, **575**, 25–31.
- 92 M. Ghaedi, A. Shokrollahi, A. H. Kianfar, A. S. Mirsadeghi, A. Pourfarokhi and M. Soylak, *J. Hazard. Mater.*, 2008, **154**, 128–134.
- 93 M. Ghaedi, A. Shokrollahi, M. R. Fathi, S. Gharaghani and M. Soylak, *Quim. Nova*, 2008, **31**, 70–74.
- 94 A. R. Rod, S. Borhani and F. Shemirani, *Eur. Food Res. Technol.*, 2006, **223**, 1438–2377.
- 95 P. Hashemi, R. Afzari, M. M. Abolghasemi and A. Olin, *Sens. Actuators, B*, 2007, **121**, 396–400.
- 96 P. Hashemi, M. M. Abolghasemi, K. Alizadeh and R. A. Zarjani, *Sens. Actuators, B*, 2008, **129**, 332–338.
- 97 P. Hashemia, M. Hosseini, K. Zargoosh and K. Alizadeh, *Sens. Actuators, B*, 2011, **153**, 24–28.
- 98 K. Saidi, W. Chaabani and M. Dammak, *RSC Adv.*, 2021, **11**, 30926–30936.
- 99 E. Antico, M. Lerchi, B. Rusterholz, N. Achermann, M. Badertscher, M. Valiente and E. Pretsch, *Anal. Chim. Acta*, 1999, **388**, 327–338.
- 100 J. N. Miller and J. C. Miller, *Statistics and Chemometrics for Analytical Chemistry*, Prentice-Hall, London, 5th edn, 2005.
- 101 A. A. Maria and W. I. Neil, *Open J. Chem.*, 2019, **5**, 30–34.

