



Cite this: *Lab Chip*, 2019, 19, 1332

A miniaturized push–pull-perfusion probe for few-second sampling of neurotransmitters in the mouse brain†

Floris T. G. van den Brink,^a Thas Phisonkunkasem,^b Ashish Asthana,^a
 Johan G. Bomer,^a Arn M. J. M. van den Maagdenberg, ^{bc}
 Else A. Tolner ^{bc} and Mathieu Odijk ^{*a}

Measuring biomolecule concentrations in the brain of living animals, in real time, is a challenging task, especially when detailed information at high temporal resolution is also required. Traditionally, microdialysis probes are used that generally have sampling areas in the order of about 1 mm², and provide information on concentrations with a temporal resolution of at least several minutes. In this paper, we present a novel miniaturized push–pull perfusion sampling probe that uses an array of small 3 μm-wide sampling channels to sample neurotransmitters at a typical recovery rate of 61%, with a reduced risk of clogging. The added feature to segment the dialysate inside the probe into small water-in-decane droplets enables the detection of concentrations with a temporal resolution of a few seconds. Here we used the probe for *in vivo* recordings of neurotransmitter glutamate released upon electrical stimulation in the brain of a mouse to demonstrate the feasibility of the probe for real-time neurochemical brain analysis.

Received 23rd October 2018,
 Accepted 1st March 2019

DOI: 10.1039/c8lc01137k

rsc.li/loc

Introduction

One major challenge in neuroscience research is to obtain reliable information on the concentration of neurotransmitters and other signalling molecules, with a high temporal resolution, at specific locations in the brain.¹ Such neurochemical knowledge can be used to unravel the complex dynamics of neuronal brain activity, not only in the healthy brain, but also in a disease context. Unfortunately, current neurochemical measurement approaches have technical limitations that hamper real-time, local assessment of these neurochemical processes.

The analysis of neurochemical molecules, such as glutamate or acetylcholine, in brain extracellular fluid is traditionally done with microdialysis,^{2,3} push–pull perfusion sampling,^{4–6} or electrochemistry,⁷ for example with arrays of biosensor electrodes located on ceramic-based ‘Gerhardt’ probes^{8,9} or silicon-based micro-arrays.¹⁰ An overview of the

benefits and disadvantages of the various methods is described in Table 1.

As discussed in a review by Kennedy,¹ microdialysis techniques suffer from a low temporal (at least several minutes) and spatial (over ~1 mm²) resolution. The smallest commercially available dialysis probes are ~200 μm in diameter with a membrane tip length of 1 mm, resulting in a sampling area of 628 000 μm² and therefore rather large compared to the size of the rodent brain.¹¹ Alternatives for localized sampling are capillary push–pull perfusion sampling (PPPS) probes^{5,6} and direct sampling using a single capillary,¹² typically with needle diameters between 90 and 360 μm and with sampling areas between 250 and 2000 μm². The poor temporal resolution is caused by target molecules arriving at different points in time at the detector, depending of their position in the parabolic flow profile inside the transporting capillary, the so-called “Taylor dispersion effect”.¹³

In an attempt to overcome some of these problems, capillary PPPS probes have been attempted that make use of microfluidic droplet generators.^{5,14,15} Combining microfluidic droplet generators – to compartmentalize the samples – with commercially available probes further improved the temporal resolution in microdialysis experiments.^{16,17} The major advantage of compartmentalization is that it limits Taylor dispersion, yet it comes at the cost of a more complex analysis afterwards. Segmented flow sampling has also been used in combination with electrospray ionization-mass spectrometry for the detection of acetylcholine *in vivo*.¹⁸

^a BIOS – Microdevices for Chemical Analysis group, MESA+ Institute for Nanotechnology, Techmed Centre, University of Twente, Hallenweg 15, 7522 NH Enschede, The Netherlands. E-mail: m.odijk@utwente.nl

^b Department of Human Genetics, Leiden University Medical Center, Einthovenweg 20, 2333 ZC Leiden, The Netherlands

^c Department of Neurology, Leiden University Medical Center, Einthovenweg 20, 2333 ZC Leiden, The Netherlands

† Electronic supplementary information (ESI) available. See DOI: 10.1039/c8lc01137k



Technology	Temporal resolution	Sampling area	Lower concentration range	Range of molecules	Remarks
Sampling probes					
Dialysis probe ^{11,20,21}	Minutes	$\geq 0.6 \text{ mm}^2$	nM	Wide	Difficult to use – risks of clogging
Push-pull perfusion probe ^{5,6,15,22}	Minutes	$\geq 0.0003 \text{ mm}^2$	nM	Wide	
Micro push-pull perfusion probe	Seconds	0.004 mm^2	nM	Wide	
Sensing probes					
Electrochemical probe ^{23,24}	Seconds	$\sim 0.003 \text{ mm}^2$	μM	Limited	Reference electrode needed

Sample analysis for both types of probes is done on-line, outside the sampling area, using a dedicated optical setup based on fluorescence detection. The optical filters and light



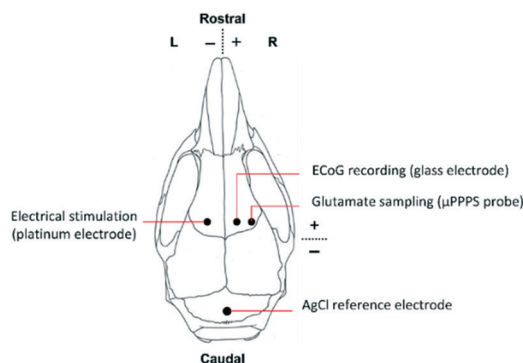


Fig. 4 Schematic representation of a mouse skull indicating locations of the μ PPPS probe in relation to the stimulation site, ECoG and reference electrode during *in vivo* experiments in an anesthetized mouse.

To promote efficient sample collection, a low negative pressure is applied to the droplet outlet. Ideally, the push-pull probe is operated in such a way that the push and pull flows are equal, which prevents withdrawing of liquid from or introducing liquid to the measurement volume (*i.e.* a sample cup, or mouse brain tissue). In practice, this is difficult to realize and the operating conditions are determined in such a way that a small inward flow is established in order to establish a stable sampling process.

An electrical equivalent circuit is used to determine the appropriate flow and pressure conditions to operate the probe and to predict the inward flow rate. Hydraulic resistances of the microfluidic channels and connected tubing, together with the flow and pressure sources are modelled in a circuit as shown in S1†. From this schematic, it can be calculated that an outlet pressure of -80 kPa, a continuous phase flow of 200 nL min $^{-1}$ and perfusion flow of 50 nL min $^{-1}$ give rise to an inwards flow rate of 126 nL min $^{-1}$.

Numerical simulations

To predict the recovery rate of both types of our μ PPPS probes, simulations were run on a 3D-model (see S10†) of the probe using COMSOL Multiphysics (version 5.3). Flow velocity (u) and pressure (p) variables were calculated using the Stokes flow approximation of the Navier–Stokes equation (creeping flow physics model) (1) and the continuity eqn (2), after which concentration (c) distributions were calculated using the steady-state convection–diffusion equation (transport of diluted species physics model, with convection and without migration) (3):

$$\mu \nabla^2 u - \nabla p = 0 \quad (1)$$

$$\nabla \cdot u = 0 \quad (2)$$

$$u \cdot \nabla c - D \nabla^2 c = 0 \quad (3)$$

The viscosity is used from water at 293 K and the mass transport is studied of a substance with $D = 0.9 \times 10^{-9}$ m 2 s $^{-1}$,

equal to the value for monosodium glutamate.³⁵ Boundary conditions are a perfusion inflow of 25 to 100 nL min $^{-1}$, and an outlet pressure between -10 kPa and -80 kPa *vs.* atmospheric pressure (1 bar or 101.32 kPa). Note that this outlet pressure is set right after the tip of the needle using a laminar outflow boundary condition, including the small hydraulic resistance, but not including the droplet generator, or connecting tubing towards the detection area. Pressure around the probe tip was set to 1 bar (atmospheric pressure). All other boundaries carry a no-slip condition ($u = 0$). An arbitrary concentration (c_0) of 1 mM was defined at the boundaries around the probe tip and of 0 mM at the perfusion inlet. We have validated that any arbitrary concentration will lead to identical results for the recovery rate, as we do not take any adsorption effects into account. The concentration gradient normal to the outlet is set to zero and the flux normal to all other boundaries is zero.

The concentration distributions at the tip are shown in Fig. 2, for a perfusion flow rate (Q_{H_2O}) of 50 nL min $^{-1}$ and an outlet pressure of either (C) -10 kPa or (D) -80 kPa. In the plot it can be seen that the sampling channels promote a significant uptake of compounds around the probe tip. To quantify this uptake, the recovery rate (the ratio between sampled concentration, and external concentration) is calculated at the channel outlet. The calculated values are plotted in Fig. 2A for varying perfusion flow rates and outlet pressures. As can be expected, the recovery rate increases if the negative outlet pressure is increased or the perfusion flow rate is decreased. To measure concentration changes at a reasonable temporal resolution, a certain inward flow is needed to provide a sufficient recovery rate. For example, the recovery rate under conditions similar to those discussed above (*i.e.* with a perfusion flow rate of 50 nL min $^{-1}$ and an outlet pressure of -80 kPa) is 88% .


Methods

Probe fabrication

The μ PPPS probes were fabricated in the Nanolab cleanroom of the MESA+ Institute of Nanotechnology, following the steps as illustrated in Fig. 3.

Silicon wafers are provided with a thermal SiO $_2$ layer, which was used as a buried mask that is patterned with the fluidic channel structures. Following a second lithography step, fluidic inlets and outlets (140 μ m) and the channel structures (20 μ m) were etched in two consecutive deep reactive ion etching (DRIE) steps. The delicate sampling channel structures are protected by a thin thermally grown oxide layer to prevent damage during the last DRIE step to release the probe. The channels were covered with a 500 μ m thick borosilicate glass wafer by anodic bonding, etched with 25% hydrogen fluoride (HF) and subsequently polished back to ~ 20 μ m thickness using chemical mechanical polishing. In the last two steps, the probes were released by etching slits through the glass and the silicon layers surrounding the structures. The probes were kept in place within the wafer



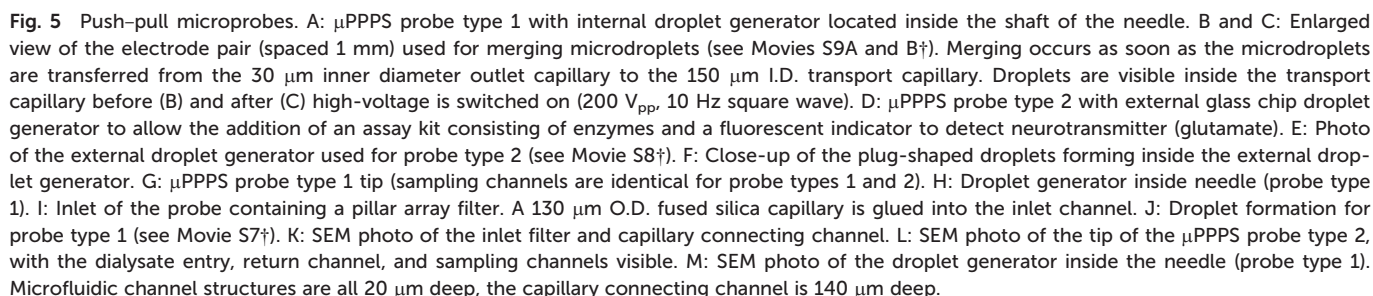

Nieuwegein, Netherlands). Some 2.5 cm of 30 μm inner diameter (ID)/130 μm outer diameter (OD) fused silica capillary tubing was glued (type NOA83H, Norland Optical Adhesives, Cranbury (NJ), USA) in the probe inlets and outlet. The NOA83H glue is UV-curable, which was used to cure the glue before it enters the microfluidic channels by capillary forces. Subsequently, the cyanoacrylate was added on this joint to

add additional bonding strength. Curing of the cyanoacrylate was sped up using a spray can of CA accelerator (Zip Kicker, ZAP, Ontario (CA), USA). The other end of the 130 μm OD tubing was subsequently glued by repeating the glue step with NOA83H and cyanoacrylate to 30 cm of 150 μm ID/360 μm OD-fused silica capillary tubing. Finally, the 360 μm OD-fused silica capillary was fixed to the polystyrene substrate using epoxy (Loctite EA M-31CL, Henkel, Nieuwegein, Netherlands). See Fig. 5A for a photo of the assembled device.

A different probe type 2 was constructed for the glutamate level measurements, because an additional inlet was needed to supply the chemicals for an enzyme-based assay. This device is shown in Fig. 5D. In this case, a push-pull microprobe without internal droplet generator is connected to a dialysate inlet. The outlet of this probe is connected with a 2.5 cm long glass capillary of 30 μm ID/130 μm OD to an external borosilicate glass droplet generator. This droplet generator contains a Y-junction where the dialysate + sample flow is combined with the enzymes and fluorophore precursor. Droplets were generated from this mixture in decane at a T-junction, and the droplet contents were subsequently mixed in a meandering channel. In the first step, 100 μm channels in this droplet generator were wet-etched (25% HF, etch rate $\sim 0.9 \mu\text{m min}^{-1}$). In the second step, 380 μm inlets were wet-etched for the glass capillaries to be glued in place.

Chemicals

Sampling with the μ PPPS probes was done by generating aqueous droplets in decane as the continuous phase. Decane has relatively low values for gas solubility compared to *e.g.* fluorinated alkanes, which prevents gas bubbles being formed inside the probe due to the negative outlet pressures.^{36,37} *In vitro* characterization was done using fluorescein that was prepared in a 10 mM stock solution and titrated in de-ionized water to sample from varying concentrations. Water was purified using an Elga PureLab flex purification system. Water and decane were filtered using a 0.22 μm pore size filter prior to use. Decane, resorufin sodium salt and fluorescein sodium salt were obtained from Sigma-Aldrich GmbH (Steinheim, Germany).

For *in vivo* recordings a sterile minimal perfusion fluid (MPF) solution, consisting of 140.3 mM NaCl, 3.0 mM KCl, 1.0 mM $\text{MgCl}_2 \cdot 6\text{H}_2\text{O}$ and 1.2 mM $\text{CaCl}_2 \cdot 2\text{H}_2\text{O}$ in MilliQ and filtered with a 0.2 μm sterilizing filter, was used for the ‘push’ flow. Glutamate measurements were performed using an Amplex Red glutamic acid/glutamate oxidase assay kit (Thermo Fisher Scientific, Breda, The Netherlands). With this method, L-glutamic acid is oxidized by glutamate oxidase to produce α -ketoglutarate, H_2O_2 and NH_3 . Subsequently, H_2O_2 reacts with Amplex Red in a 1 : 1 ratio catalysed by horseradish peroxidase to generate resorufin, a highly fluorescent product.

Measurement setup

The microprobe was mounted in a custom-made holder and connected to a syringe pump (Nemesys, Cetoni GmbH,

Korbussen, Germany) to infuse dialysate and decane. A pressure pump (MFCS-EZ, Fluigent, Paris, France) was used to apply negative pressure for sampling. For the electrical merging of droplets, a waveform generator (Agilent 33250A, Santa Clara, USA) was connected to an amplifier with an amplification of 100 V/V (Trek model 2210, Trek Inc., Lockport (NY), USA). To monitor the applied signal, an Agilent DSO3062A oscilloscope (Santa Clara, USA) was installed. For droplet merging pictures, a stereomicroscope with a PTGREY grasshopper 3 camera (FLIR Integrated Imaging Solutions GmbH, Ludwigsburg, Germany) was used. The droplets recorded inside the probe needle were recorded with an inverted Olympus microscope (Hamburg, Germany) with the same grasshopper 3 camera.

The optical setup consists of a high-power LED (M530L3, Thorlabs, Munich, Germany) controlled by a LED driver (LEDD1B, Thorlabs). LED power was measured using a silicon photodiode (S121C, Thorlabs) connected to a power meter (PM100USB, Thorlabs). The LED was focused at a measurement tube, which is a 50 μm ID/360 μm OD glass capillary tube from which the polyimide coating is locally removed. Alignment and focus of the LED beam was verified using a CMOS camera (DCC1545M, Thorlabs). For fluorescence measurements, a right-angle mirror (DFM/M-P01, Thorlabs) was used to reflect the beam towards a photomultiplier tube (PMT) (H7422, Hamamatsu, Herrsching am Ammersee, Germany). The PMT signal was amplified with 1 V μA^{-1} using an amplifier unit (C7319, Hamamatsu) before being collected by a National Instruments myDAQ board (Woerden, Netherlands). See Fig. S2A[†] for more information on the measurement setup and a schematic overview of the optics.

In vivo recordings

For the *in vivo* experiments in a mouse brain, first, the fluorescent signal intensity was calibrated *in vitro* using a 0 μM , 5 μM and 10 μM glutamate solution, since the expected glutamate levels in the mouse cortex are between approximately 2 and 5 μM .²⁴ Since auto-oxidation of Amplex Red and deterioration of glutamate oxidase are known problems with this assay kit, this calibration procedure was performed every day. Moreover, with these concentration steps the time delay between sampling and detection is measured as well, allowing one to link the timing of measured fluorescence signal to the cortical activity changes occurring in the brain.

Subsequently, the mouse was prepared for *in vivo* surgery for measuring cortical glutamate levels (Fig. S5B†). Animals used for the experiments were male C57BL/6J mice (Harlan, Venray, The Netherlands), kept under standard housing conditions with a 12 hour light/dark cycle with free access to water and food. All animal experiments were approved by local (LUMC Authority of Animal Welfare) and national (Central Authority for Scientific Procedures on Animals) ethical committees in accordance with recommendations of the European Communities Council Directive (2010/63/EU). All efforts

After setting up this experiment, a recovery and baseline recording period of 15 minutes was observed, or longer in case signals had not stabilized. Next, transcallosal electrical stimulation was performed using the bipolar microelectrode on the left hemisphere (contralateral to the EcoG recording

The raw glutamate signal obtained from the PMT was processed using Matlab (version R2017a, Mathworks Inc., Natick, MA, USA), first to remove all data points below the baseline background fluorescence, second, to apply a moving averaging filter of 500 points (equal to 0.5 seconds). The AC ECoG signal recorded on the second channel of the MyDAQ was obtained from the glass electrode using a 3rd order Butterworth band-pass filter with cut-offs at 0.5 and 200 Hz.

Probe fabrication

Electrodes connected to the transport capillary to fuse droplets to prevent dispersion of smaller droplets can be seen in Fig. 5A–C. Microscopy images of key features of the probe are shown in Fig. 5G–I. The purple coloring in the microscopy images arises from the silicon oxide passivation layer inside the channels. In Fig. 5G and L, the tip of the needle with its sampling channels is shown. Fig. 5H and J shows an inset of the middle part of the needle.

Droplet formation

First the possibility to generate droplets was tested for the two probe types (see Fig. 5J for type 1, and 5E and F for type 2). In Fig. 5J, droplet formation is visualized for a probe with the droplet generator embedded in the needle tip. In this experiment, the flow rate of oil was set to 200 nL min^{-1} , perfusion with demineralized water was set to 50 nL min^{-1} , and the outlet pressure was set to -50 kPa . From the high-speed video (400 frames per second (fps)), it was estimated that droplets were generated at a rate of 80 fps (see Movie S7†).

For the second probe type, a push–pull probe is connected to an external droplet generator that enables the mixing of a sample containing the neurotransmitter glutamate with glutamate oxidase (GLOx), horseradish peroxidase (HRP) and a fluorophore precursor (Amplex Red) to obtain a glutamate concentration-dependent fluorescent signal. This arrangement is shown in Fig. 5D–F. Here, the flow rate of decane was set to 500 nL min^{-1} , the flow rate of the GLOx/HRP/Amplex Red mixture was set to 200 nL min^{-1} , perfusion of DI water was set to 100 nL min^{-1} and the outlet pressure was set to -50 kPa . Droplets are generated on average at a rate of 1 drop per second (see Movie S8†).

As soon as the microdroplets generated in probe type 1 are transferred from the outlet capillary to the much wider transport capillary, they form a dense packing at first (see Fig. 5B), but due to the parabolic flow velocity profile, droplets moving along the centerline will be faster than those closer to the wall again causing dispersion. Therefore, measurements will get distorted because the order of the droplets moving through the optical detector will be different from the order in which they were generated. As a result, the temporal resolution goes down to ~ 1 minute, as shown in Fig. S3A.† To solve this, a pair of electrodes was installed right after the outlet capillary in order to electrically merge microdroplets into larger ones that fit the dimensions of the transfer capillary, thereby forming a stable segmented flow and preserving the temporal resolution of the concentration variations in the sample (see Fig. 5C).

Based on separate measurements of the generation rate and volume of the small and merged droplets, it is estimated that about 50 droplets are merged into one bigger droplet (see Movies S9A and B†). Although the segmented flow was restored by this merging step, theoretically this modification will reduce the temporal resolution only by the ratio of the original and merged droplet generation rates, which is estimated to be a factor of 50.

Optical detection

The uPPPS probes are designed to sample neurotransmitter from the brain, which will be detected using fluorescence

spectroscopy. Our optical setup is designed for resorufin detection, which is a fluorescent dye used in a variety of commercially available assay kits (see S2† for more details).

To demonstrate the possibility to detect resorufin at a sufficiently low concentration, the optical setup is first characterized with respect to the limit of detection for resorufin sodium salt. Fig. 6 shows a linear response in the lower concentration range of resorufin from 2 to 20 nM. Analysis of the recorded signal from the photomultiplier tube (PMT) reveals that the limit of detection (LOD) of this system can be estimated to be about 2 nM, which corresponds to 3 times the standard deviation of the blank value (see Fig. S2B†). Note that this LOD is reported for resorufin to determine the lower limitations of the optical setup. Basal glutamate levels in the brain are typically 3 orders of magnitude larger fluctuating around a few μM .³⁸

In vitro sampling

Next, the sampling capability of probe type 1 was verified using fluorescein sodium salt. An aqueous stock solution of 10 mM fluorescein was prepared and a titration experiment was done in a 10 mL sample cup with a magnetic stirrer (500 rpm). Flow rates of 200 nL min⁻¹ decane, 50 nL min⁻¹ perfusion with demineralized water were used, and the outlet pressure was set to -80 kPa. Stepwise addition of 200 μL of stock solution with intervals of 100 seconds resulted in the fluorescence intensity plot of Fig. 7A. LED power was set to 300 μW.

For glutamate measurements using the type 2 probe, a commercial assay kit based on glutamate oxidase and the fluorescent marker resorufin was used. The design of the μ PPPS probes does not allow for the addition of the enzymes and amplex red to the droplets, and adding these to the dialysate flow before the sampling area is undesirable for obvious reasons. Therefore, the push-pull probe with external droplet generator was fabricated, which allows one to add the components of the assay kit to the sample flow just before the droplet-generating T-junction. Analogous to the fluorescein titration experiment, a 10 mL sample cup was used with $1\times$ PBS and a magnetic stirrer (500 rpm). A stepwise addition of 20 μ L of 1 mM L-glutamate with intervals of 100 seconds resulted in the fluorescence intensity plot of Fig. 7C. Flow rates were set to 500 nL min^{-1} decane, 200 nL min^{-1} GLOx/HRP/Amp. Red mixture, 100 nL min^{-1} perfusion with sterile perfusion fluid and an outlet pressure of -50 kPa was used. A typical titration curve for fluorescein is indicated in Fig. 7A, and is representative of comparable curves obtained from a total of $n = 3$ experiments (see S3B†). From this curve it can be seen that a sudden increase of approximately 180 μM in concentration can be measured within 3 seconds. This delay of 3 seconds can be explained in part by the time needed for the added fluorescein to mix in the sample cup, and in part by the Taylor dispersion occurring in the needle between sampling channels and droplet generator. The relation between fluorescein concentration and fluorescent readout is calculated by an algorithm that cuts off any data-point below

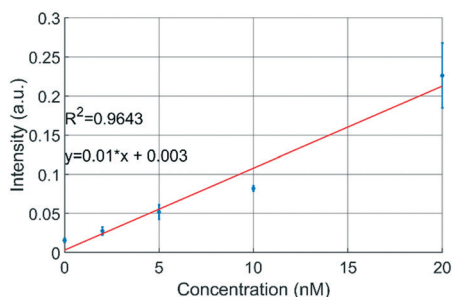


Fig. 6 Fluorescence measurements with resorufin sodium salt demonstrate that concentrations <2 nM can be measured using the developed optical detection setup (see text for details). Resorufin was injected directly into the optical detection capillary ($n = 3$).

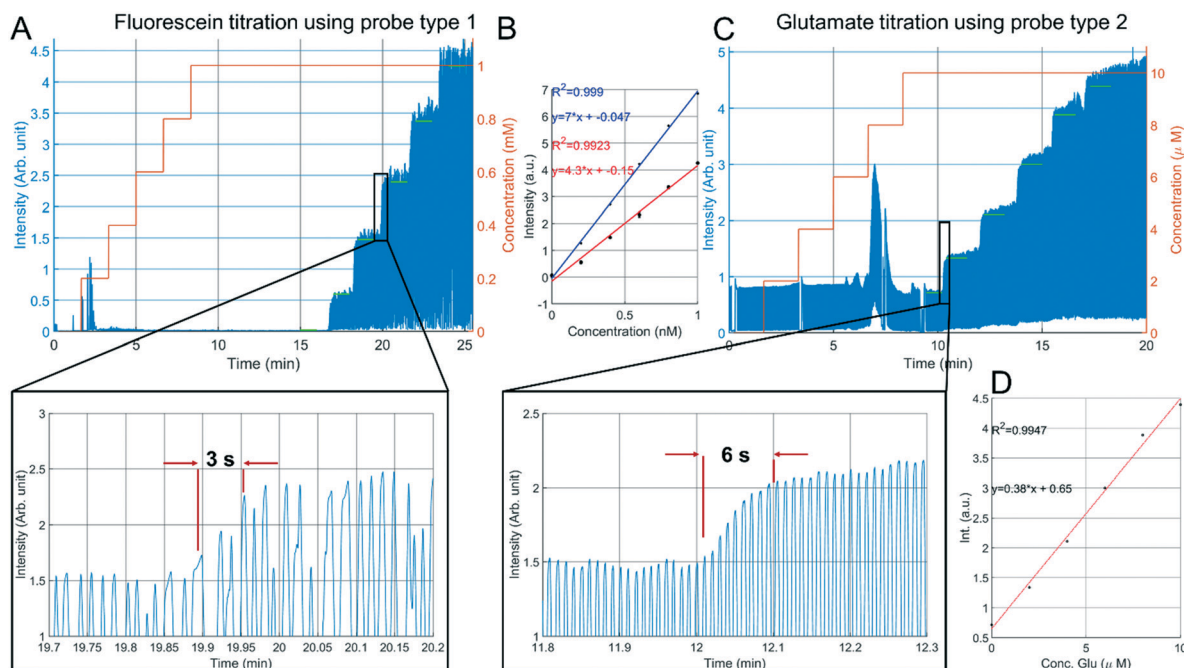


Fig. 7 *In vitro* sampling from a 10 mL sample cup. A: Stepwise addition of fluorescein sampled with a probe type 1 having a droplet generator embedded in the needle. B: Relation between fluorescent readout and fluorescein concentration (red fitting curve) ($n = 3$), extracted from the green plateaus from the titration curves of Fig. 7A and S3B†. The blue line indicates a calibration curve with fluorescein directly infused into the detection capillary. C: Stepwise addition of glutamate sampled with a probe type 2 having an external droplet generator in which glutamate oxidase, horseradish peroxidase and Amplex red are added. In the presence of glutamate, Amplex red is converted to highly fluorescent resorufin. The peaks at 2.5 min (Fig. 7A) and 7.5 min (Fig. 7B) are residual fluorophore resulting from earlier conducted staircase experiments. D: Relation between fluorescent readout and glutamate concentration, extracted from the green plateaus indicated in Fig. 7B.

a minimum threshold that is 80% of the maximum plateau value. Comparing the intensity values measured for the droplets ($n = 3$) to a calibration curve recorded at the same LED power (see Fig. 7B), the recovery rate is estimated at 61%. However, as can be seen from the insets in Fig. 7, the fluorescent signal from the droplets never reach a plateau value. It is therefore not unlikely to assume that the real recovery rate might be even higher.

Glutamate titration using the probe type 2 (Fig. 7C) showed a slower response, roughly double the rise time observed with fluorescein. In addition to the time required for the glutamate to mix in the sample cup, the longer transfer distance between the tip of the probe and the external droplet generator causes some extra Taylor dispersion that adds to the total response time. Nonetheless, our results indicate that the compartmentalization in droplets are a significant improvement compared to the several minute time scale results shown using traditional dialysis probes combined with either flow injection analysis,²⁰ or fluorescent readout in continuous flow.²¹

The relation between glutamate concentration and fluorescent readout is calculated in an identical manner as for the fluorescein experiments. The algorithm cuts off any data-point below a minimum threshold that is 80% of the maximum plateau value. Next, the mean of each plateau (green lines in Fig. 7C) is calculated, as shown in Fig. 7D. The sensitivity is $0.38 \text{ a.u. } \mu\text{M}^{-1}$. Additional experiments ($n = 2$ in S4†)

showed similar results, albeit with slightly different sensitivities of 0.45 and $0.30 \text{ a.u. } \mu\text{M}^{-1}$. Linearity was good with R^2 values between 0.9918 and 0.9969 . A small offset is present at zero concentration, this could be due to known issues of self-formation of resorufin in the absence of glutamate with the Amplex Red assay kit.³⁹ Based on the calibration curves shown in Fig. 7D and S4† it is expected that our setup should be sensitive enough to detect both basal levels (few μM) and bursts of glutamate ($\sim 40 \mu\text{M}$) *in vivo*.^{24,38} Compared to the fluorescein titrations, reproducibility was lower for experiments conducted with the glutamate assay kit, which was largely due to variable enzyme activities across (purchased) batches. The glutamate assay kit is sensitive to small changes in temperature during the droplet transfer, and to a lesser degree small variations in timing between the start of the reaction and the optical readout. Moreover, if resorufin is in direct contact with the walls of the channel adsorption can occur, leading to drift in the fluorescence intensity measurements.

In vivo recordings

To demonstrate that the μ PPPS probes are not only working in an *in vitro* environment, but are also functional in *in vivo* experiments, we used probe type 2 with external droplet generator to record changes in glutamate levels in the brain of an anesthetized mouse. As a proof of principle, such changes



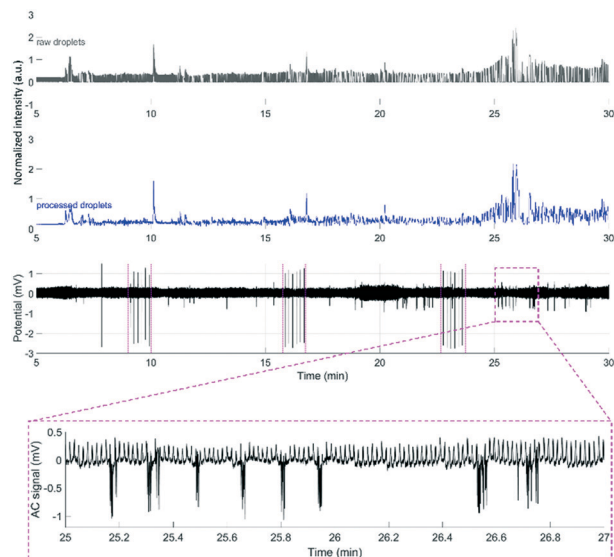


Fig. 8 Example recordings of glutamate during an *in vivo* experiment using the μ PPPS probe with external droplet generator for measuring neurotransmitter glutamate changes during evoked cortical activity by electrical stimulation on the left sensorimotor cortex (periods including the stimulus pulses, visible on the ECoG trace, are indicated by magenta-colored dashed lines around 9, 17 and 23 minutes) in an anesthetized mouse. See Fig. 6 for a schematic of the experimental approach. Shown are the normalized raw optical droplet read-out (grey) from the right sensorimotor cortex, the processed droplet signal (blue), and alternating current (AC) (black) local field potential “electrocorticogram” (ECoG) recordings from a glass electrode inserted in superficial layers of the right sensorimotor cortex. For the first two stimulation sessions, the glutamate signal shows a transient increase directly following cortical stimulation, whereas in the third session the glutamate signal increased with a delay, in line with a pronounced burst of cortical activity that is evident on the AC ECoG recording (see additional inset showing details of the AC response at higher time resolution).

were recorded in the right sensorimotor cortex while cortical activity was evoked in the right sensorimotor cortex using transcallosal electrical stimulation in the left hemisphere^{40,41} (see Fig. 8). It has been demonstrated by others that increased cortical network activity is paralleled by increased extracellular levels of glutamate *in vivo*.^{42,43} Experiments were successfully performed in two mice, in which an electrical stimulation paradigm was repeated three times. Each stimulation paradigm consisted of a set of 6 biphasic 1 ms pulses at 70% of the maximum cortical response, delivered at 0.1 Hz. The resulting glutamate responses, as well as the recordings from a standard glass electrode are shown in Fig. 8. A simple staircase recording, similar to what is shown in Fig. 7 was conducted prior to insertion of the probe in the brain to check for proper functioning of the setup. From the delay observed between *in vitro* addition of glutamate and time of detection, the delay time was estimated to be approximately 4.25 minutes. This approximate delay time was used in *post hoc* analysis for shifting the droplet trace to the left (in case of the example in Fig. 8 by a shift of 4.25 minutes). Fig. 8 shows representative traces from one of the mouse experi-

ments, with subsequent electrical stimulation of brain activity and related changes in fluorescent signal, as measured by the μ PPPS probe, indicative of altered cortical glutamate levels. In the shown example, fluorescent signals from the sampled droplets increased following cortical electrical stimulation, either directly (at 10 and 17 min), or with a delay (25 min), in line with pronounced cortical burst activity (see inset). Observations are in line with expected rises in cortical glutamate levels during the evoked cortical activity.

Conclusions and outlook

Here we have demonstrated the design and fabrication of a miniaturized push-pull perfusion sampling probe with a width of 140 μm and a height of 140 μm . Molecules (including neurotransmitters) enter the probe through 20 small sampling channels ($20 \times 3 \mu\text{m}^2$) located at the end of the probe, effectively providing a sampling area of approximately 1200 μm^2 . A recirculating, U-shaped channel in the tip of the needle, operated in a push-pull-like fashion ensures fast transport of sample to the in-house developed external measurement setup. The detection method used for the *in vitro* and *in vivo* glutamate experiments in this study is based on fluorescence spectroscopy using a sensitive photomultiplier tube, and (in combination with μPPPS probes of type 2) the mixing of externally generated droplet samples with glutamate oxidase and fluorophore precursor Amplex Red. The detection limit for the fluorescent reaction product of the Amplex Red assay kit, resorufin, in our experiments was $\sim 2 \text{ nM}$. Immediately after sampling, the dialysate is encapsulated into water-in-decane droplets to prevent dispersion, and to enhance the temporal resolution. *In vitro* experiments using a solution containing fluorescein demonstrated a recovery rate of 61%, while step-wise changes in concentration could be measured within 3 seconds. As proof of principle, transient changes in brain glutamate levels were recorded *in vivo* in the cortex of anesthetized mice that were electrically stimulated on the contralateral cortical hemisphere. These experiments demonstrated a correlation between evoked cortical network activity and enhanced glutamate release, as indicated by rises in fluorescent signal.

Whereas our *in vivo* pilot data are encouraging, there is still a challenge with the μ PPPS probe and fluorescent measurement approach. Small variations in droplet generation rate (in the order of a couple of seconds at most), which could occur due to technical changes in the fluidic system, will cause small fluctuations in the timing between brain activity changes and our detection of droplet signals, which can result in a larger cumulative variation due to the relatively long time between sampling and detection (4–5 minutes). This issue can be solved by detecting neurotransmitters immediately inside the body of the probe. This could be done optically (as we used in our study for detection outside of the probe), but, based on unpublished results from our team, it should also be possible to measure glutamate by electrochemical means inside droplets. In that scenario, inclusion

of a separate channel for calibration fluids would allow periodic recalibration of such electrochemical measurements. An additional benefit offered by switching to a different detection method is to prevent the issues observed with the glutamate assay kit obtaining reproducible activity, which make the glutamate assay kit not suitable for quantitative measurements.

In our current design we did not include additional functionality (*e.g.* measuring electrical activity) to the glass cover of the probe during fabrication. As we have shown in previous work,²³ it would be relatively straightforward to also include AC- and/or DC-EEG electrodes to create a hybrid probe that combines microfluidic sampling with brain activity recordings. Moreover, it would be feasible in the future to also include waveguides to enable optogenetic stimulation.

Conflicts of interest

There are no conflicts to declare.

Acknowledgements

STW is gratefully acknowledged for funding this VENI project (grant no. 13607). The Netherlands Organ-on-Chip Initiative (NOCI), a Gravitation project (024.003.001) is acknowledged, funded by the Netherlands Wetenschaps Organisatie (NWO). We thank Jan van Nieuwkastele for help with optics and camera recordings, Hans de Boer for assistance with the optical suitcase and probe positioner, Vasilis Papadimitriou for help with capturing the droplet formation on video, Karin Groothuis-Oudshoorn (University of Twente) and Jelle Goeman (Leiden University Medical Center) for their assistance with data statistics. The authors would like to thank Dr. Pieter Roelfsema (Dutch Brain Institute) and Gunnar Flik (Charles River Laboratories, Groningen) for fruitful discussions.

References

- 1 R. T. Kennedy, *Curr. Opin. Chem. Biol.*, 2013, **17**, 860–867.
- 2 T. I. F. H. Cremers, M. G. de Vries, K. D. Huinink, J. P. van Loon, M. v d Hart, B. Ebert, B. H. C. Westerink and E. C. M. De Lange, *J. Neurosci. Methods*, 2009, **178**, 249–254.
- 3 C. J. Watson, B. J. Venton and R. T. Kennedy, *Anal. Chem.*, 2006, **78**, 1391–1399.
- 4 N. A. Cellar, S. T. Burns, J. C. Meiners, H. Chen and R. T. Kennedy, *Anal. Chem.*, 2005, **77**, 7067–7073.
- 5 T. R. Slaney, J. Nie, N. D. Hershey, P. K. Thwar, J. Linderman, M. A. Burns and R. T. Kennedy, *Anal. Chem.*, 2011, **83**, 5207–5213.
- 6 S. Kottegoda, I. Shaik and S. A. Shippy, *J. Neurosci. Methods*, 2002, **121**, 93–101.
- 7 S. Qin, M. van der Zeyden, W. H. Oldenzien, T. I. F. H. Cremers and B. H. C. Westerink, *Sensors*, 2008, **8**, 6860–6884.
- 8 B. K. Day, F. Pomerleau, J. J. Burmeister, P. Huettl and G. A. Gerhardt, *J. Neurochem.*, 2006, **96**, 1626–1635.
- 9 R. T. Kennedy, *Anal. Chem.*, 2016, **88**, 1230–1237.
- 10 Y. Kim, H. J. Lee, D. Kim, Y. K. Kim, S. H. Lee and E. Yoon, in *Transducers conference*, 2013, pp. 876–879.
- 11 R. Rathnasingham, D. R. Kipke, S. C. Bledsoe and J. D. McLaren, *IEEE Trans. Biomed. Eng.*, 2004, **51**, 138–145.
- 12 M. Perry, Q. Li and R. T. Kennedy, *Anal. Chim. Acta*, 2009, **653**, 1–22.
- 13 E. R. Hascup, K. N. Hascup, M. Stephens, F. Pomerleau, P. Huettl, A. Gratton and G. A. Gerhardt, *J. Neurochem.*, 2010, **115**, 1608–1620.
- 14 M. D. Johnson, R. K. Franklin, M. D. Gibson, R. B. Brown and D. R. Kipke, *J. Neurosci. Methods*, 2008, **174**, 62–70.
- 15 J. Voipio, M. Pasternack and K. Macleod, in *Microelectrode techniques, The Plymouth workshop handbook*, ed. D. Ogden, The company of Biologists, Cambridge UK, 2nd edn, 1994, pp. 275–316.
- 16 E. Bakker, P. Bühlmann and E. Pretsch, *Chem. Rev.*, 1997, **97**, 3083–3132.

- 33 J. P. Seymour, F. Wu, K. D. Wise and E. Yoon, *Microsyst. Nanoeng.*, 2017, 3, 16066.
- 34 F. van den Brink, A. Asthana, J. Bomer, E. Tolner, A. van den Maagdenberg and M. Odijk, *21st Int. Conf. Miniaturized Syst. Chem. Life Sci.*, 2017, pp. 215–216.
- 35 A. C. F. Ribeiro, M. M. Rodrigo, M. C. F. Barros, L. M. P. Verissimo, C. Romero, A. J. M. Valente and M. A. Estesio, *J. Chem. Thermodyn.*, 2014, 74, 133–137.
- 36 L. N. Mizerovsky and K. P. Smirnova, *Russ. Chem. Bull.*, 2010, 59, 673–676.
- 37 A. M. A. Dias, R. P. Bonifácio, I. M. Marrucho, A. A. H. Pádua and M. F. Costa Gomes, *Phys. Chem. Chem. Phys.*, 2003, 5, 543–549.
- 38 J. J. Burmeister and G. A. Gerhardt, *Anal. Chem.*, 2001, 73, 1037–1042.
- 39 B. Zhao, F. A. Summers and R. P. Mason, *Free Radical Biol. Med.*, 2012, 53, 1080–1087.
- 40 G. Tsenov and P. Mareš, *Physiol. Res.*, 2007, 56, 485–491.
- 41 E. A. Tolner, D. W. Hochman, P. Hassinen, J. Otáhal, E. Gaily, M. M. Haglund, H. Kubová, S. Schuchmann, S. Vanhatalo and K. Kaila, *Epilepsia*, 2011, 52, 104–114.
- 42 M. H. Millan, T. P. Obrenovitch, G. S. Sarna, S. Y. Lok, L. Symon and B. S. Meldrum, *Epilepsy Res.*, 1991, 9, 86–91.
- 43 L. Medina-Ceja, K. Pardo-Peña, A. Morales-Villagrán, J. Ortega-Ibarra and S. López-Pérez, *BMC Neurosci.*, 2015, 16(1), 11.

