



Cite this: *RSC Adv.*, 2019, 9, 28207

Ultra-small dispersed Cu_xO nanoparticles on graphene fibers for miniaturized electrochemical sensor applications†

Jinfeng Zeng,^a Xiaoteng Ding,^b Liwei Chen,^a Le Jiao,^a Yuze Wang,^a Christopher D. Windle,^c Qing Han ^{*a} and Liangti Qu ^a

A graphene microfiber (GF) modified with ultrafine Cu_xO nanoparticles (Cu_xONPs/GF) has been fabricated by direct annealing of electrodeposited nano-sized copper-based metal organic frameworks (HKUST-1) and used as an electrode for nonenzymatic H₂O₂ sensing. Benefiting from the unique microfiber architecture and synergetic effects, as well as strong coupling between components with many active sites and boosted electron transport, the Cu_xONPs/GF electrode shows prominent sensitivity, selectivity and long-term operational stability for the detection of H₂O₂. Further work successfully applied this Cu_xONPs/GF electrode to detection of H₂O₂ in real samples such as milk and human serum. These results indicate that the Cu_xONPs/GF is a promising mini-sized sensor in electrochemical analysis.

Received 20th May 2019
 Accepted 28th August 2019

DOI: 10.1039/c9ra03802g

rsc.li/rsc-advances

Introduction

The demand for electrochemical sensors with high sensitivity, low cost, excellent selectivity, and facile miniaturization has stimulated extensive research into developing versatile materials with remarkable electrocatalytic activity. Compared to conventional macro-electrodes,¹ fiber-type electrodes with a one-dimensional microstructure, particularly carbon fiber microelectrodes possessing one dimensional diffusion, have been widely fabricated and used in sensors due to their low cost, small volume, portability and good biocompatibility. However, the poor electrocatalytic activity and low current response of carbon fiber microelectrodes seriously restrict their application in sensing.

Graphene has potential as an electrode for electrochemical analysis owing to its large specific surface area, excellent electron mobility, high mechanical properties and good biocompatibility. Recently, we reported a graphene fiber assembled with chemically reduced graphene sheets, which exhibited promising electrochemical sensing activity, mainly owing to the inherent defects and residual oxygenated functional groups as active sites. However, the weak electrocatalytic properties of graphene restrict its wide application in electrochemical

analysis. It is revealed that combining graphene fiber with catalytically active nanomaterials such as metals and metal oxides is an efficient way to enhance the electrocatalytic activity.^{2–12} Copper oxide nanoparticles (Cu_xONPs) are an attractive alternative electroactive species due to their abundance, low cost, good chemical stability and unique electronic properties.^{13,14} Hybridizing graphene with Cu_xONPs is an effective way, where the composite materials have fully exploited the structural merits of individual components and improved the analytic performance. So far, various strategies, including thermal conversion,¹⁵ ion exchange,¹⁶ wet chemistry,¹⁷ microwave,¹⁸ template growth,¹⁹ and anion-assisted approaches²⁰ have been employed to prepare Cu_xONPs/graphene hybrids. Unfortunately, as-prepared Cu_xONPs from these approaches suffer from aggregation on graphene-based materials, leading to poor dispersion and a low number of active sites with poor electrocatalytic performance. In addition, although Cu_xONPs/graphene composites have been widely investigated and demonstrated with great potential for electrochemical analysis, there is still a lack of exploration for its miniaturized sensors. Thus, it is urgent to design and develop a simple and effective method for the production of Cu_xONPs/graphene fiber-based microsensor with a high number of active sites and highly efficient electrocatalytic activity.

Hydrogen peroxide (H₂O₂) is indispensable to ecosystems and is widely used in foodstuffs, the environment, medicine and industry. Excess H₂O₂ can lead to toxicity for humans and to the environment.^{21–24} Although electrochemical enzyme-based sensors have good selectivity and high performance, their applications are limited because of their poor stability and high cost. Therefore, the development of non-enzymatic sensors has drawn tremendous attention. Herein, we report

^aKey Laboratory of Photoelectronic/Electrophotonic Conversion Materials, Key Laboratory of Cluster Science, Ministry of Education of China, School of Chemistry and Chemical Engineering, Beijing Institute of Technology, Beijing 100081, P. R. China. E-mail: qhan@bit.edu.cn

^bCollege of Life Sciences, Qingdao University, Qingdao 266071, P. R. China

^cSolar Energy and Advanced Materials Group, Department of Chemical Engineering, University College London, Torrington Place, London, WC1E 7JE, UK

† Electronic supplementary information (ESI) available: Additional Fig. S1–S7, Tables S1 and S2, and more discussions. See DOI: 10.1039/c9ra03802g



a graphene microfiber electrode modified by well-dispersed and ultrafine Cu_xO nanoparticles ($\text{Cu}_x\text{ONPs}/\text{GF}$) derived from copper-based metal organic frameworks (HKUST-1) by a direct electrodeposition self-assembly technique for nonenzymatic electrochemical H_2O_2 detection. The unique nanoarchitecture and synergetic effect as well as strong coupling between components endows them with a high density of active sites and enhanced electron transport leading to improved electrochemical micro-sensing. The resulting hybrid fiber electrode exhibits a very low detection limit of $0.023 \mu\text{M}$ and a rapid response time of 1 s. Our work provides a straightforward method for synthesizing highly efficient nonenzymatic micro-sensing electrodes for H_2O_2 detection.

Experimental

Synthesis of graphene fiber (GF)

Graphene oxide (GO) was synthesized by oxidation of graphite powder according to the modified Hummers' method.²⁵ Then, graphene oxide fibers (GOF) were prepared by a wet spinning strategy. Typically, 3 mL GO (20 mg mL^{-1}) was spun into a methanol solution saturated by potassium chloride (KCl) with a speed of 0.1 m s^{-1} by an injector (with a diameter of 0.25 mm), followed by drying. To obtain GF, the GOF was heated to $200 \text{ }^\circ\text{C}$ for 2 h at first and then further heated to $1000 \text{ }^\circ\text{C}$ for 2 h with a heating rate of $10 \text{ }^\circ\text{C min}^{-1}$ under N_2/H_2 ($v/v = 4 : 1$) atmosphere.

Synthesis of HKUST-1 nanoparticles decorated GF (HNPs/GF)

A two-electrode system was used for the preparation of HNPs/GF (HNPs = HKUST-1 nanoparticles). Firstly, 0.2416 g of cupric nitrate trihydrate ($\text{Cu}(\text{NO}_3)_2 \cdot 3\text{H}_2\text{O}$), 0.2102 g of 1,3,5-benzenetricarboxylic acid (H_3BTC) and 0.7748 g of tetrabutylammonium hexafluorophosphate (NBu_4PF_6) were dispersed in 20 mL of *N,N*-dimethylformamide (DMF) solution, and the mixture was treated by ultrasound for 30 min to obtain a homogeneous solution. Next, the as-synthesized GF (2.0 mm length) and a commercial Pt plate were used as the working electrode and counter electrode, respectively. The HNPs/GF was fabricated by the electrodeposition of HNPs on the GF surface in the above mixed solution (degassed with N_2 for 30 min) at -1.5 V for 60 s, the obtained sample is denoted $\text{HNPs}_{60}/\text{GF}$. For comparison, a series of HNPs/GF samples with different amounts of HNPs were obtained by adjusting the electrodeposition time (30 s, 90 s, and 120 s) in the same mixed solution, which were denoted $\text{HNPs}_{30}/\text{GF}$, $\text{HNPs}_{90}/\text{GF}$ and $\text{HNPs}_{120}/\text{GF}$, respectively.

Synthesis of $\text{Cu}_x\text{ONPs}/\text{GF}$

The $\text{Cu}_x\text{ONPs}/\text{GF}$ was synthesized by direct annealing of HNPs/GF ($\text{HNPs}_{30}/\text{GF}$, $\text{HNPs}_{60}/\text{GF}$, $\text{HNPs}_{90}/\text{GF}$ and $\text{HNPs}_{120}/\text{GF}$) samples from room temperature to $400 \text{ }^\circ\text{C}$ in N_2 with a ramp rate of $10 \text{ }^\circ\text{C min}^{-1}$ and stabilized for 2 h, then cooled to room temperature naturally, and denoted $\text{Cu}_x\text{ONPs}_{30}/\text{GF}_{400}$, $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$, $\text{Cu}_x\text{ONPs}_{90}/\text{GF}_{400}$ and $\text{Cu}_x\text{ONPs}_{120}/\text{GF}_{400}$, respectively.

In order to study the influence of the annealing temperature on the performance of the final samples, a series of $\text{Cu}_x\text{ONPs}/\text{GF}$ samples were obtained by annealing the $\text{HNPs}_{60}/\text{GF}$ sample at $300 \text{ }^\circ\text{C}$ and $500 \text{ }^\circ\text{C}$, respectively. The obtained samples were denoted $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{300}$ and $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{500}$, respectively.

Synthesis of $\text{Cu}_x\text{ONPs}/\text{GF}$ electrode

The $\text{Cu}_x\text{ONPs}/\text{GF}$ was glued with silver conductive adhesive onto stainless steel sheets ($2.5 \times 0.5 \text{ cm}$). The end of the tip was sealed with molten paraffin. The exposed $\text{Cu}_x\text{ONPs}/\text{GF}$ was cut down to 2.0 mm in length and used as the electrode. The exposed stainless steel sheet was then connected with the electrochemical workstation.

Results and discussion

The procedure for the fabricated $\text{Cu}_x\text{ONPs}/\text{GF}$ is shown in Fig. 1. Firstly, GO suspension (Fig. 1a) was converted into a GO fiber (GOF, Fig. 1b) by a wet spinning strategy. After drying naturally, the GOF was thermally reduced to graphene fiber (GF, Fig. 1c). The obtained GF with a diameter of $44 \mu\text{m}$ appears as wrinkled sheet-like surface morphologies (Fig. S1†). Then, electrodeposition self-assembly of the copper MOF (HKUST-1 nanoparticles, HNPs) occurred in a mixed solution containing cupric nitrate trihydrate ($\text{Cu}(\text{NO}_3)_2 \cdot 3\text{H}_2\text{O}$) and 1,3,5-benzenetricarboxylic acid (H_3BTC), in which HNPs grew *in situ* on the surface of GF after 60 s of electrodeposition ($\text{HNPs}_{60}/\text{GF}$, Fig. 1d), which was confirmed by X-ray diffraction (XRD, Fig. S2†). As shown in Fig. 2a, the obtained $\text{HNPs}_{60}/\text{GF}$ shows fiber features with a diameter of $45 \mu\text{m}$, larger than that of the bare GF. Fig. 2b demonstrates that the HNPs_{60} with an octahedral structure have a uniform size of 200 nm and are well distributed over the surface of GF. Further annealing at $400 \text{ }^\circ\text{C}$ led to pyrolysis of HNPs_{60} with simultaneous formation of Cu_xO

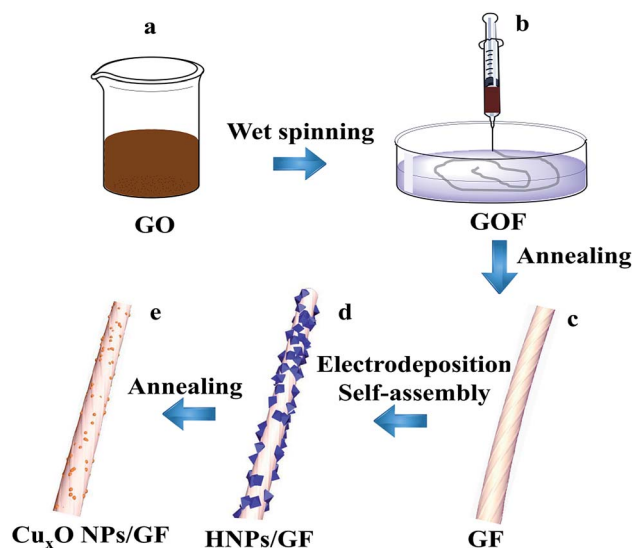


Fig. 1 Schematic illustration of the preparation of $\text{Cu}_x\text{ONPs}/\text{GF}$. (a) GO solution, (b) GOF, (c) GF, (d) HNPs/GF, (e) $\text{Cu}_x\text{ONPs}/\text{G}$.



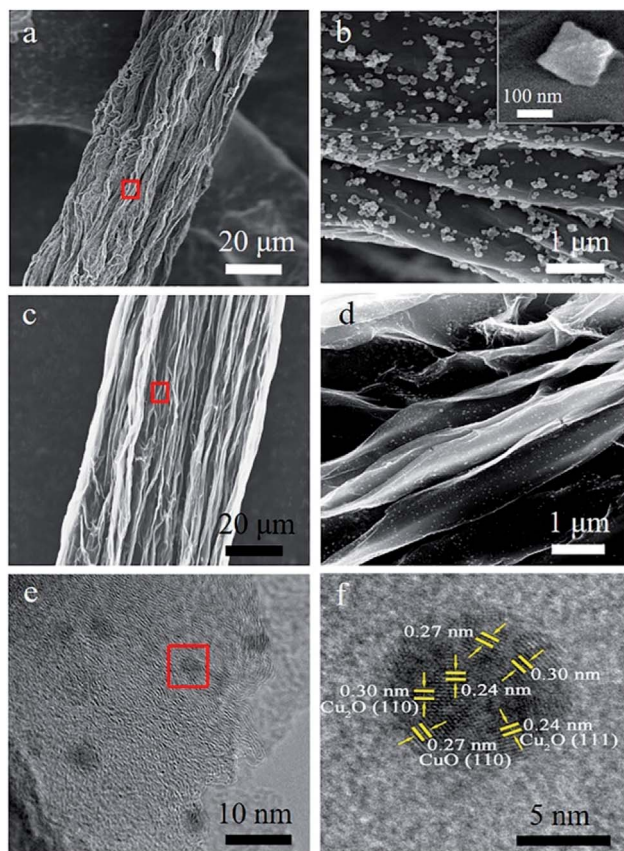


Fig. 2 (a) Scanning electron microscopy (SEM) images of HNP₆₀/GF. (b) The enlarged view of the rectangle area in (a). The inset in (b) is an enlarged SEM image of a single HNP₆₀. (c) SEM image of Cu_xONPs₆₀/GF₄₀₀. (d) The enlarged view of the rectangle area in (c). (e) Transmission electron microscopy (TEM) image of sheets within the Cu_xONPs₆₀/GF₄₀₀. (f) The enlarged view of the rectangle area in (e).

nanoparticles (Cu_xONPs₆₀, the size is about 10 nm) well distributed on the sheets of GF (Cu_xONPs₆₀/GF₄₀₀, Fig. 2c–e). High-resolution transmission electron microscopy (HR-TEM) of Cu_xONPs/GF (Fig. 2f) indicates clear lattice fringes with a spacing of 0.24, 0.27 and 0.30 nm, corresponding to the Cu₂O(111), CuO(110) and Cu₂O(110), respectively.^{26–30} Element mapping reveals the coexistent and uniform distribution of C, O and Cu elements for Cu_xONPs₆₀/GF₄₀₀ (Fig. 3a). An X-ray

photoelectron spectrum (XPS) of the bare GF shows C 1s (284.6 eV) and O 1s (531.2 eV) peaks. Apart from the C 1s and O 1s peaks observed in the GF, the Cu_xONPs₆₀/GF₄₀₀ shows the two apparent Cu 2p_{3/2} and Cu 2p_{1/2} features at 934.2 eV and 944.4 eV with a Cu atomic percentage of 0.76% (Fig. 3b), indicating the presence of Cu_xONPs₆₀, which is consistent with the energy-dispersive X-ray spectroscopy measurement (EDS, Fig. S3 and Table S1†). The ratio of C/O decreases from 11.1 (GF) to 8.4 (Cu_xONPs₆₀/GF₄₀₀), demonstrating an increase in the oxygen content resulting from the introduction of Cu_xO. In addition, the chemical states of copper in Cu_xONPs₆₀/GF₄₀₀ are revealed by the high-resolution XPS spectra (Fig. 3c). The signals of Cu 2p_{3/2} and Cu 2p_{1/2} can each be deconvoluted into two peaks of Cu₂O (933.4 eV and 935.4 eV) and CuO (941.9 eV and 944.2 eV)³¹ ascribed to the oxidation products of HNPs after annealing.

H₂O₂-sensing properties

The electrochemical properties of the Cu_xONPs₆₀/GF₄₀₀ electrode are investigated in 0.1 M PBS saturated with N₂ at a scan rate of 50 mV s⁻¹. Considering the electrodeposition self-assembly time has a significant effect on the content and size of Cu_xONPs, as well as the catalytic performance of the Cu_xONPs/GF electrode, various Cu_xONPs/GF electrodes were obtained by adjusting the electrodeposition self-assembly time (30 s, 90 s and 120 s), which were denoted Cu_xONPs₃₀/GF₄₀₀, Cu_xONPs₉₀/GF₄₀₀, and Cu_xONPs₁₂₀/GF₄₀₀, respectively. The SEM images and EDS analysis of the Cu_xONPs/GF samples (Fig. S4 and Table S1†) imply that with the increasing time of electrodeposition self-assembly, the content and size of the Cu_xONPs increase. As a result, there is almost no reductive peak at the Cu_xONPs₃₀/GF₄₀₀ electrode (Fig. 4a), which can be attributed to only trace amounts of Cu_xO with inferior electrocatalytic activity (Fig. S4a and b and Table S1†). In comparison, an obviously reductive peak (about -0.05 V) was observed for the Cu_xONPs₆₀/GF₄₀₀ electrode, which was attributed to the successful electrode surface reaction process.

A further increase of electrodeposition self-assembly time causes severe agglomeration of Cu_xONPs with a reduction in the number of active sites (Fig. S4e–h†) resulting in a decrease in the current response. The annealing temperature also has a significant effect on the size of Cu_xONPs and performance of

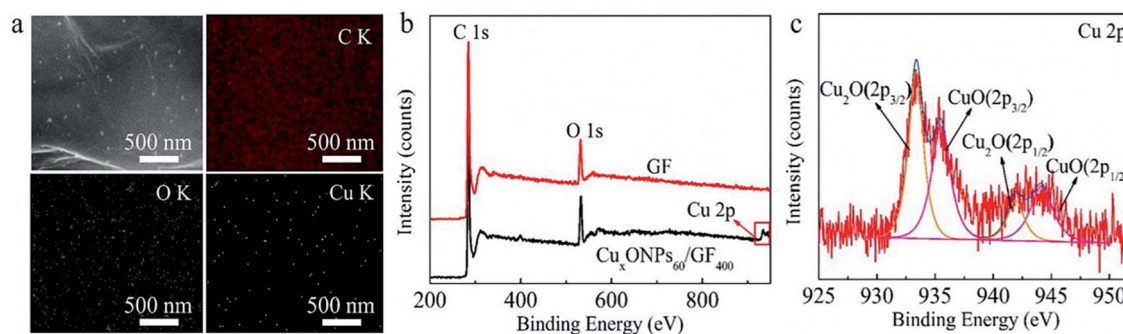


Fig. 3 (a) Scanning transmission electron microscopy (STEM) and C-, O- and Cu-element mappings for the sheets within the Cu_xONPs₆₀/GF₄₀₀. (b) XPS spectra of the Cu_xONPs₆₀/GF₄₀₀ and the bare GF. (c) High-resolution Cu 2p XPS spectrum of Cu_xONPs₆₀/GF₄₀₀.



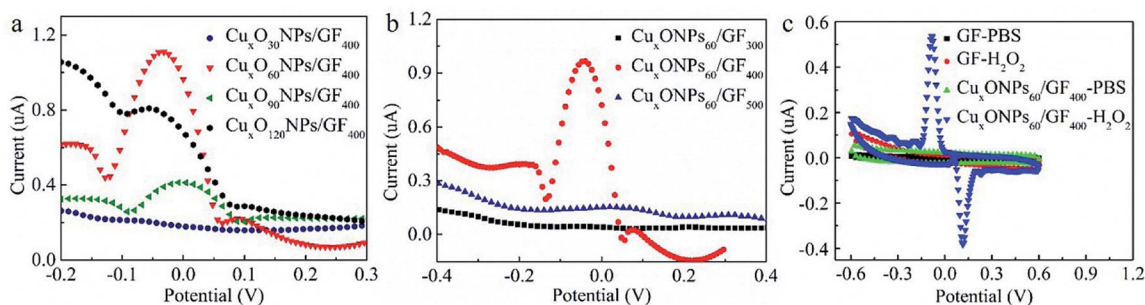


Fig. 4 (a) Differential pulse voltammograms (DPVs) of the $\text{Cu}_x\text{ONPs}_{30}/\text{GF}_{400}$, $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$, $\text{Cu}_x\text{ONPs}_{90}/\text{GF}_{400}$ and $\text{Cu}_x\text{ONPs}_{120}/\text{GF}_{400}$ in 0.1 M phosphate buffer solution (PBS) with 0.2 mM H_2O_2 (pH = 7.15). (b) DPVs of the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{300}$, $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ and $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{500}$ in 0.1 M PBS with 0.2 mM H_2O_2 (pH = 7.15). (c) Cyclic voltammograms (CVs) of the bare GF and the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrodes in 0.1 mM PBS (pH = 7.15) without and with 0.2 mM H_2O_2 .

the final $\text{Cu}_x\text{ONPs}/\text{GF}$ electrode. For comparison, a series of $\text{Cu}_x\text{ONPs}/\text{GF}$ electrodes were prepared by annealing the precursors of HNP/GF derived from the optimal electrodeposition time at different temperatures (300 °C and 500 °C, which were denoted $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{300}$ and $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{500}$, respectively). Apparently, the current response signal of the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode is obviously higher than that of the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{300}$ and the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{500}$ electrodes (Fig. 4b). This may be attributed to the incomplete decomposition of the HNP₆₀ precursor for the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{300}$ electrode (Fig. S5a†). The residual non-conductive HNP₆₀ inhibit electron transport on the surface of GF, leading to poor electrocatalytic activity towards H_2O_2 sensing. For the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{500}$ electrode, an increase of $\text{Cu}_x\text{ONPs}_{60}$ size can be observed as shown in Fig. S5b,† hence reducing the utilization of active sites and leading to a decrease in electrocatalytic performance.³²

As a result, compared with the bare GF (no redox peaks, Fig. 4c), the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode displays a couple of sharp redox peaks, indicating an excellent electrocatalytic activity of the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode towards H_2O_2 detection. Meanwhile, the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode shows an obvious reduction peak at pH = 7.15 (Fig. S6†), which means that the electrode can be applied to a physiological environment. The low detection limit and the linear range of the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode for H_2O_2 were measured by differential pulse voltammetry (DPV). As shown in Fig. 5a, the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode displays two linear responses for H_2O_2 detection with a good sensitivity of $56.25 \mu\text{A mM}^{-1} \text{cm}^{-2}$ and a low detection limit of $0.023 \mu\text{M}$ in the range of $0.07\text{--}1.13 \mu\text{M}$ (Fig. 5b), whilst displaying an ultrahigh sensitivity of $3437.5 \mu\text{A mM}^{-1} \text{cm}^{-2}$ in the range of $1.20\text{--}133 \mu\text{M}$ (Fig. 5c). The reason for two linear relationships herein was probably caused by the different H_2O_2 absorption and activation on the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode catalyst under different H_2O_2 concentrations.³² At extremely low H_2O_2 concentration, the electrocatalytic process is dominated by H_2O_2 absorption, but at high H_2O_2 concentration, the process is dominated by H_2O_2 activation. Accordingly, the low detection limit obtained at the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode was estimated to be $0.023 \mu\text{M}$ (S/N = 3). As a contrast, the sensing performances of recently reported H_2O_2 sensors based on copper-based electrodes are shown in Table

S2.†^{32–41} Detection limit of $0.023 \mu\text{M}$ and linear range of $0.07\text{--}133 \mu\text{M}$ achieved by using the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$. The overall performance of $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ exceed the most of copper-based electrodes, which benefiting from the unique

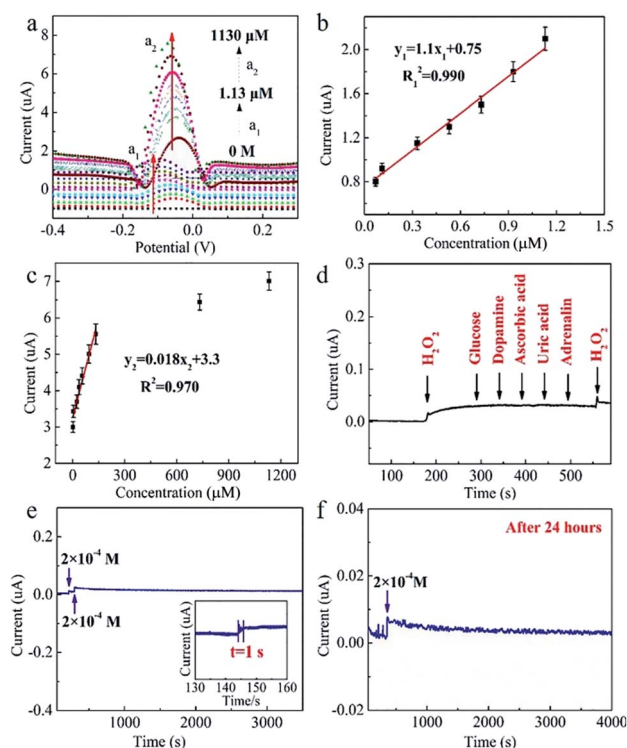


Fig. 5 (a) DPVs of the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode in PBS (pH = 7.15) of various H_2O_2 concentrations. The concentration of H_2O_2 is from $0.07 \mu\text{M}$ to 1.13mM , scan rate: 50mV s^{-1} . (b) The fitting curves of reductive current vs. concentration of H_2O_2 ($0.07, 0.09, 0.11, 0.13, 0.33, 0.53, 0.73, 0.93, 1.13 \mu\text{M}$). (c) The fitting curve of current response vs. H_2O_2 concentration ($1.2, 5.2, 9.2, 13.2, 53.2, 93.2, 133, 733, 1130 \mu\text{M}$). (d) Amperometric responses of $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ electrode at potential of -0.15V in the 0.1 M PBS with 0.2 mM H_2O_2 , 0.04 mM glucose, 0.04 mM dopamine, 0.04 mM ascorbic acid, 0.04 mM uric acid and 0.04 mM adrenalin. (e) Amperometric curve of the $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ consistently adding 0.2 mM H_2O_2 under gentle agitation. (f) The amperometric curve of the same $\text{Cu}_x\text{ONPs}_{60}/\text{GF}_{400}$ after 24 h with addition of 0.2 mM H_2O_2 .



Table 1 Determination of H₂O₂ in real samples at the Cu_xONPs₆₀/GF₄₀₀ microelectrode ($n = 3$)

Sample	Added (μM)	Founded (μM)	Recovery (%)	Repeatability (% RSD)
Milk	0.47	0.49	104.3	4.01
	0.60	0.58	96.7	3.15
	5.30	5.39	101.7	3.08
	94.10	94.83	100.8	2.15
Human Serum	0.47	0.48	102.1	3.34
	0.60	0.57	95.0	2.08
	5.30	6.11	115.3	4.10
	94.10	95.06	101.0	4.05

microfiber architecture and synergetic effect as well as strong coupling between components with countless active sites and boosted electrons transport. In addition, few group attempt for electrochemical detection of H₂O₂ on fiber electrode.

The selectivity test of the Cu_xONPs₆₀/GF₄₀₀ electrode was carried out in 0.1 M phosphate buffer solution (PBS). 0.2 mM H₂O₂ was added, followed by 0.04 mM glucose, 0.04 mM dopamine, 0.04 mM ascorbic acid, 0.04 mM uric acid and 0.04 mM adrenalin, respectively. As shown in Fig. 5d, after adding 0.2 mM H₂O₂, a distinct current response was observed, and there was almost no change in the peak current in the presence of the interferents. In addition, when a further 0.2 mM H₂O₂ was added, the current signal showed the same response as after the first H₂O₂ addition, indicating the excellent selectivity of the Cu_xONPs₆₀/GF₄₀₀ electrode. The Cu_xONPs₆₀/GF₄₀₀ electrode shows a response time of H₂O₂ detection within 1 s, indicating it tracks very quickly (Fig. 5e inset). The peak current barely changed after 3500 s (Fig. 5e), and after storing at room temperature for 24 h, the response signal of the Cu_xONPs₆₀/GF₄₀₀ electrode remains 98% of its original response for H₂O₂ detection (Fig. 5f), revealing a good operational stability of the Cu_xONPs₆₀/GF₄₀₀ electrode.

Detection of H₂O₂ in milk and human serum

The Cu_xONPs₆₀/GF₄₀₀ electrode was used for the determination of 0.47, 0.60, 5.30, and 94.10 μM H₂O₂ in diluted milk and diluted human serum samples (Table 1 and Fig. S7 and S8[†]), respectively. The recovery rates calculated according to the calibration curves (Fig. 5b and c) were 104.3%, 96.7%, 101.7% and 100.8% for milk, and 102.1%, 95.0%, 115.3% and 101.0% for human serum, respectively, the relative standard deviation were less than 4.10% for $n = 3$, indicating that the Cu_xONPs₆₀/GF₄₀₀ electrode is effective for H₂O₂ detection in a biological system.

Conclusions

In summary, we have fabricated a graphene fiber electrode modified with well-dispersed and superfine copper oxide nanoparticles derived from electrodeposition self-assembly of a copper-based metal organic frameworks. The as-prepared Cu_xONPs/graphene fiber electrode exhibits a high number of

active sites and enhanced electrode exhibits a high number of active sites and enhanced electron-transfer ability. It shows highly efficient electro-catalytic activity for nonenzymatic electrochemical H₂O₂ detection, greater than any previously reported Cu_xONPs-based electrodes. This work provides a simple method for the rapid production of a novel fiber electrode for electrochemical sensor applications.

Conflicts of interest

There are no conflicts to declare.

Acknowledgements

This work was supported by the NSFC (21575014, 21905025), Beijing Natural Science Foundation (2184122), the Fundamental Research Funds for the Central Universities (2018CX01017), Beijing Institute of Technology Research Fund Program for Young Scholars, the project of State Key Laboratory of Explosion Science and Technology (Beijing Institute of Technology, YBKT18-03), and Analysis & Testing Center, Beijing Institute of Technology.

References

- 1 J. Zhang, J. Han, Z. Shi, Y. Ju, Z. Zhang and M. Gu, *Appl. Surf. Sci.*, 2019, **465**, 357–361.
- 2 L. Gao, J. Zhuang, L. Nie, J. Zhang, Y. Zhang, N. Gu, T. Wang, J. Feng, D. Yang, S. Perrett and X. Yan, *Nat. Nanotechnol.*, 2007, **2**, 577.
- 3 Z. Zhang, J. Hao, W. Yang, B. Lu, X. Ke, B. Zhang and J. Tang, *ACS Appl. Mater. Interfaces*, 2013, **5**, 3809–3815.
- 4 F. Natalio, R. André, A. F. Hartog, B. Stoll, K. P. Jochum, R. Wever and W. Tremel, *Nat. Nanotechnol.*, 2012, **7**, 530.
- 5 P. Pengo, S. Polizzi, L. Pasquato and P. Scrimin, *J. Am. Chem. Soc.*, 2005, **127**, 1616–1617.
- 6 W. Shi, X. Zhang, S. He and Y. Huang, *Chem. Commun.*, 2011, **47**, 10785–10787.
- 7 W. Chen, J. Chen, A. L. Liu, L. M. Wang, G. W. Li and X. H. Lin, *ChemCatChem*, 2011, **3**, 1151–1154.
- 8 X. X. Wang, Q. Wu, Z. Shan and Q. M. Huang, *Biosens. Bioelectron.*, 2011, **26**, 3614–3619.
- 9 P. Roy, Z. H. Lin, C. T. Liang and H. T. Chang, *Chem. Commun.*, 2012, **48**, 4079–4081.
- 10 Z. Chen, J. J. Yin, Y. T. Zhou, Y. Zhang, L. Song, M. Song, S. Hu and N. Gu, *ACS Nano*, 2012, **6**, 4001–4012.
- 11 M. Baghayeri, H. Alinezhad, M. Tarahomi, M. Fayazi, M. Ghanei-Motlagh and B. Maleki, *Appl. Surf. Sci.*, 2019, **478**, 87–93.
- 12 J. Cai, S. Ding, G. Chen, Y. Sun and Q. Xie, *Appl. Surf. Sci.*, 2018, **456**, 302–306.
- 13 K. Zhang, N. Zhang, H. Cai and C. Wang, *Microchim. Acta*, 2012, **176**, 137–142.
- 14 L. Lu and X. Huang, *Microchim. Acta*, 2011, **175**, 151–157.
- 15 J. Huang, Y. Zhu, H. Zhong, X. Yang and C. Li, *ACS Appl. Mater. Interfaces*, 2014, **6**, 7055–7062.



- 16 L. Zhou, L. Kuai, W. Li and B. Geng, *ACS Appl. Mater. Interfaces*, 2012, **4**, 6463–6467.
- 17 R. Agarwal, K. Verma, N. K. Agrawal, R. K. Duchaniya and R. Singh, *Appl. Therm. Eng.*, 2016, **102**, 1024–1036.
- 18 C. Yang, X. Su, F. Xiao, J. Jian and J. Wang, *Sens. Actuators, B*, 2011, **158**, 299–303.
- 19 X. Zhang, S. Sun, J. Lv, L. Tang, C. Kong, X. Song and Z. Yang, *J. Mater. Chem. A*, 2014, **2**, 10073–10080.
- 20 C. Kong, L. Tang, X. Zhang, S. Sun, S. Yang, X. Song and Z. Yang, *J. Mater. Chem. A*, 2014, **2**, 7306–7312.
- 21 Y. Sun, M. Luo, Y. Qin, S. Zhu, Y. Li, N. Xu, X. Meng, Q. Ren, L. Wang and S. Guo, *ACS Appl. Mater. Interfaces*, 2017, **9**, 34715–34721.
- 22 Y. Hu, Z. Zhang and C. Yang, *Anal. Chim. Acta*, 2007, **601**, 95.
- 23 X. Zhu, X. Niu, H. Zhao and M. Lan, *Sens. Actuators, B*, 2014, **195**, 274–280.
- 24 M. Zhang, Y. Wang, L. Huang, Z. Xu, C. Li and G. Shi, *Adv. Mater.*, 2016, **27**, 6708–6713.
- 25 V. Gupta, P. Mahbub, P. N. Nesterenko and B. Paull, *Anal. Chim. Acta*, 2018, **1005**, 81–92.
- 26 A. A. M. Abdurhman, Y. Zhang, G. Zhang and S. Wang, *Anal. Bioanal. Chem.*, 2015, **407**, 8129–8136.
- 27 M. L. Huffman and B. J. Venton, *Analyst*, 2009, **134**, 18–24.
- 28 Y. T. Liao, Y. Y. Huang, H. M. Chen, K. Komaguchi, C. H. Hou, J. Henzie, Y. Yamauchi, Y. Ide and K. C. W. Wu, *ACS Appl. Mater. Interfaces*, 2017, **9**, 42425–42429.
- 29 M. Zhang, Y. Wang, L. Huang, Z. Xu, C. Li and G. Shi, *Adv. Mater.*, 2015, **27**, 6708–6713.
- 30 T. Baran, S. Wojtyła, C. Lenardi, A. Vertova, P. Ghigna, E. Achilli, M. Fracchia, S. Rondinini and A. Minguzzi, *ACS Appl. Mater. Interfaces*, 2016, **8**, 21250–21260.
- 31 X. Sun, S. Guo, Y. Liu and S. Sun, *Nano Lett.*, 2012, **12**, 4859–4863.
- 32 W. Meng, S. Xu, L. Dai, Y. Li, J. Zhu and L. Wang, *Electrochim. Acta*, 2017, **230**, 324–332.
- 33 F. Xu, M. Deng, G. Li, S. Chen and L. Wang, *Electrochim. Acta*, 2013, **88**, 59–65.
- 34 H. Song, C. Ma, L. You, Z. Cheng, X. Zhang, B. Yin, Y. Ni and K. Zhang, *Microchim. Acta*, 2015, **182**, 1543–1549.
- 35 B. B. Jiang, X. W. Wei, F. H. Wu, K. L. Wu, L. Chen, G. Z. Yuan, C. Dong and Y. Ye, *Microchim. Acta*, 2014, **181**, 1463–1470.
- 36 M. Liu, R. Liu and W. Chen, *Biosens. Bioelectron.*, 2013, **45**, 206–212.
- 37 C. Zhang, M. Wang, L. Liu, X. Yang and X. Xu, *Electrochem. Commun.*, 2013, **33**, 131–134.
- 38 S. Li, Y. Zheng, G. W. Qin, Y. Ren, W. Pei and L. Zuo, *Talanta*, 2011, **85**, 1260–1264.
- 39 Y. K. Hsu, Y. C. Chen and Y. G. Lin, *Appl. Surf. Sci.*, 2015, **354**, 85–89.
- 40 A. Gu, G. Wang, J. Gu, X. Zhang and B. Fang, *Electrochim. Acta*, 2010, **55**, 7182–7187.
- 41 J. Huang, Y. Zhu, H. Zhong, X. Yang and C. Li, *ACS Appl. Mater. Interfaces*, 2014, **6**, 7055–7062.

