



Cite this: *RSC Adv.*, 2020, 10, 28437

Selective extraction and determination of aromatic amine metabolites in urine samples by using magnetic covalent framework nanocomposites and HPLC-MS/MS

Jingjing Yu, * Bing Wang, Junlan Cai, Quanping Yan, Sheng Wang, Ge Zhao, Junwei Zhao, Lining Pan and Shaofeng Liu*

Purification and selective enrichment of ultra-low level metabolites in bio-samples is very important for HPLC-MS/MS analysis. A magnetic covalent organic framework (*i.e.* COFs) (TpPa-1) (*i.e.* 2,4,6-trihydroxybenzene-1,3,5-tricarbaldehyde-*p*-phenylenediamine) material was synthesized and used for a magnetic solid phase extraction (MSPE) method in aromatic amine (AA) metabolites (*i.e.* 1-naphthylamine, 2-naphthylamine, 3-aminobiphenyl and 4-aminobiphenyl) in urine, and then HPLC-MS/MS was employed for analysis. The morphology, pore structure, surface area, chemical composition, magnetic properties, and thermal stability of the synthesized magnetic COFs were characterized with several analysis techniques, such as nitrogen adsorption-desorption isotherms, HRTEM, FTIR, XRD, and so on. MSPE conditions were optimized and analytical performance of the developed method was characterized. The limit of detection (LOD) and limit of quantification (LOQ) of four AAs ranged from 0.01 to 0.07 ng mL⁻¹ and 0.04 to 0.22 ng mL⁻¹, respectively. The recoveries of 1-NA, 2-NA, 3-ABP, 4-ABP were in the range of 81.9–105%, 87.8–102%, 101–120%, 88.3–117%, respectively. Good intra-day and inter-day precision were obtained with RSD of less than 5.8% and 9.9%, respectively. Furthermore, the synthesized magnetic COFs absorbent could be recycled in MSPE at least 5 times. Analytical results of AA metabolites in real urine samples with the developed method showed significant difference ($p < 0.01$) between smokers and nonsmokers. Thus, urinary AA metabolites could be exposure biomarkers for cigarette smoke.

Received 7th May 2020
Accepted 17th July 2020

DOI: 10.1039/d0ra04096g

rsc.li/rsc-advances

1. Introduction

The FDA established a list of harmful and potentially harmful constituents in tobacco products and tobacco smoke in 2012.¹ It contains a series of aromatic amine (AA) compounds, such as 1-naphthylamine (1-NA), 2-naphthylamine (2-NA) and 4-aminobiphenyl (4-ABP). What's more, 2-NA and 4-ABP belong to Group 1 ("carcinogenic to humans") classified by the International Agency for Research on Cancer (IARC), while 1-NA is in Group 3 ("not classifiable as to its carcinogenicity to humans").² It has been reported that tobacco smoking is a major cause of bladder cancer^{3–5} in humans without occupational exposure, such as industries involving dyes, pharmaceuticals, pesticides and plastics, while AAs and their derivatives were important chemical intermediates.^{6–8} Urinary AAs could be used as exposure biomarkers of tobacco smoke. Some research has indicated that urinary AAs are higher in smokers than in nonsmokers.^{4,5,9,10}

AA metabolites can covalently bind to tissue macromolecules (proteins) and DNA to form adducts.^{4,5,11} And then the free, acetylated and glucuronidated AAs excreted in urine.¹¹ Thus, as for the analysis of urinary AAs, acid, base, or enzyme hydrolysis process were used for deconjugating firstly.^{4,5,9,10} Owing to the ultra-low levels of AA metabolites in urine and the complexity of urine matrix, some approaches involving complex sample cleanup or derivatization^{4,5,11} were applied before GC-MS,^{4,5} GC-MS/MS^{10,11} or HPLC-MS/MS⁹ analysis. Derivatization reaction with AAs should be conducted for GC-MS or GC-MS/MS analysis due to the higher polarity of AAs. HPLC-MS/MS has been shown to be an efficient technique avoiding derivatization for the determination of polar compounds, such as AAs. Various sample clean-up procedures were applied for different sample matrix, such as conventional liquid-liquid extraction,¹² solid-phase extraction (SPE) with SPE column^{9,13} and so on. For example, Saha's group¹² have used HPLC-MS/MS technique to determine 6 AAs in cigarette smoke, and a liquid-liquid extraction and concentration process were applied, which was tedious and time-consuming. Our group⁹ has reported that a polycyclic aromatic hydrocarbons (PAHs)-molecular

Zhengzhou Tobacco Research Institute of CNTC, Zhengzhou 450001, China. E-mail: yujingjing307@163.com; sfliu@126.com; Fax: +86-371-67672575/2055; Tel: +86-371-67672575 ext. 2055



imprinting polymer (MIP) solid extraction column was used for the determination of AAs metabolite in urine samples of smokers and nonsmokers. The PAHs-MIP column could effectively purify the urine samples and decrease the matrix effect. However, the commercial SPE column was expensive and could not be recycled.

Recently, covalent organic frameworks (COFs) materials have been widely used as solid extraction adsorbent due to their fascinating properties including high specific surface area, excellent thermal stability, high porosity.^{14–20} Magnetic solid-phase extraction (MSPE) has attracted increasing attention due to its high extraction efficiency and recycled property. MSPE technique based on COFs materials is a perfect combine and has been successfully used in sample clean-up procedure.^{21–28} For example, Wang and coworkers²¹ reported a COF-based magnetic adsorbent for solid extraction of PAHs, and HPLC was employed for quantification. The COF-LZU1@PEI@Fe₃O₄ displayed high extraction efficiency for PAHs, which was mainly attributed to strong π - π stacking and hydrophobic interaction. Chen and coworkers²² used a core-shell structured magnetic COFs for MSPE for bisphenols from human serum samples. The developed method was fast, simple, highly efficient and sensitive, and the Fe₃O₄@COF nanocomposites exhibited excellent reusability.

In the present work, a magnetic COFs (TpPa-1) composite was prepared for MSPE technique, and then used for the extraction of AAs metabolite in urine. The as-prepared magnetic COFs material were characterized with different analysis techniques, such as nitrogen adsorption-desorption isotherm, high resolution transmission electron microscopy (HRTEM), X-ray diffraction analyses (XRD) and small angle X-ray scattering (SAXS), and so on. The conditions of MSPE were optimized and analytical performance was characterized. What's more, the reusability of as-prepared magnetic COFs material was studied in this work. Four AAs (*i.e.* 1-NA, 2-NA, 3-ABP and 4-ABP) in urine were determined and their urinary excretion levels for smokers and nonsmokers were investigated as well.

2. Materials and methods

2.1. Chemicals and reagents

1-NA, 2-NA, 3-ABP, 4-ABP, 1-NA-*d*₇, 2-NA-*d*₇, 3-ABP-*d*₉ and 4-ABP-*d*₉ were analytical standard and obtained from Dr. Ehrenstorfer (purity \geq 98%, Germany). Acetonitrile and methanol were HPLC grade and purchased from Dikama Corp. (USA). Formic acid was HPLC grade and obtained from TEDIA Company Inc. (USA). Hydrochloric acid and sodium hydroxide were of analytical reagent and obtained from ACROS ORGANICS (USA). Aqueous ammonia was of analytical reagent (CNW Technologies, Germany). All other reagents were analytical standard. Water was purified with a Milli-Q system (Millipore, Bedford, MA, USA).

FeCl₃·6H₂O (97%) was ACS reagent from Sigma-Aldrich (USA), ethylene glycol (99.9%) was purchased from KEMIOU Chemical Reagents Ltd. (Tianjin, China). Anhydrous sodium acetate with purity of 99% was obtained from Alfa Aesar (USA). 1,6-Diaminohexane (98%) was obtained from Sigma-Aldrich (USA). 2,4,6-Trihydroxybenzene-1,3,5-tricarbaldehyde (Tp, 95%) was obtained from Ark Pharm, Inc. (United States). *p*-

Phenylenediamine (Pa-1, 99%) was purchased from J&K Scientific Ltd. (China). Other reagents were analytical reagent, such as dimethylformamide and 95% ethyl alcohol.

2.2. Synthesis of amino-functionalized magnetic Fe₃O₄ nanoparticles

The amino-functionalized magnetic Fe₃O₄ nanoparticles were prepared by hydrothermal reaction.²⁹ FeCl₃·6H₂O (4.0 g), anhydrous sodium acetate (8.0 g) and 1,6-diaminohexane (26.0 g) were added into ethylene glycol (120 mL) under mechanical agitation at 50 °C for 0.5 h until homogeneous solution was obtained. The mixture was added in Teflon-line stainless-steel autoclave, and sustained for 6 h at 200 °C. After the mixture was transferred into a flask, the synthesized amino-functionalized magnetic Fe₃O₄ nanoparticles was separated with the help of a magnet, and washed with water and 95% ethanol. The obtained magnetic nanoparticles dried in the air for 4 to 8 hours, and then dried in vacuum oven at 50 °C for 12 h.

2.3. Synthesis of magnetic COFs material

The synthesis of magnetic COFs (TpPa-1) material was based on Schiff-base mechanism^{30,31} and the synthetic route was as follows. 0.0630 g Tp (0.30 mmol) was dissolved in a certain volume of ethanol (10–40 mL) by stirring. And then 0.1050 g the synthesized amino-functionalized magnetic Fe₃O₄ nanoparticles was added into the Tp solution, and then under mechanical agitation at 50 °C for 0.5 h. 0.0486 g Pa⁻¹ (0.45 mmol) was dissolved in the same volume of ethanol as above (*i.e.* 10–40 mL). The obtained Pa-1 solution was added into the Tp mixture drop by drop for about 15 min under mechanical agitation in room temperature. The reaction was sustained for 12 h, and the brown colored magnetic COFs (TpPa-1) material was obtained.

The obtained mixture was dried under vacuum at 50 °C, and then washed with dimethylformamide, 95% ethanol, and methanol successively. After each step, the synthesized magnetic nanoparticles could be collected from the mixture with the help of a magnet. The obtained magnetic COFs material was dried in vacuum oven at 50 °C for 12 h.

The synthesis process of COFs material (TpPa-1) was similar to that of magnetic COFs material, except for the addition of magnetic NH₂-Fe₃O₄ nanoparticles.

2.4. Material characterization

Tristar II 3020 Surface Area Analyzer (Micromeritics Instrument Ltd. USA) was applied to obtain surface area and pore size distribution of the synthesized materials. The organo-functional group of the synthesized materials was characterized with Fourier transform infrared spectrometer (FTIR, BRUKER TENSOR 27, Germany). High resolution transmission electron microscopy (HRTEM, USA FEI TECNAI G2 F20) was used for the morphology characterization of the synthesized materials. X-ray diffraction analyses (XRD, Germany Bruker D8 venture) and small angle X-ray scattering (SAXS, Germany Bruker SAXS Nanostart) were used to characterize constitute and structure of the synthesized materials. The vibrating sample magnetometer (VSM) was used for magnetic sample


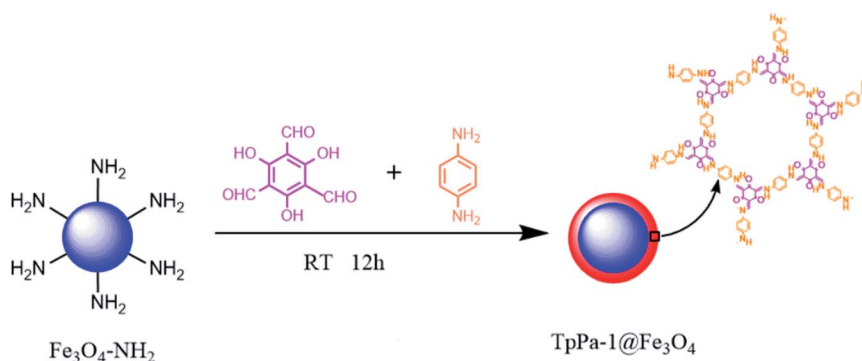


Table 1 The specific parameters of AAs and internal standards for MRM analysis

Compounds	Precursor ion (m/z)	Production Ion (m/z)	Dwell time (ms)	CE (eV)	DP (V)
1-NA	144.0	127.0 ^a /77.0	50	30	100
2-NA	144.0	127.0 ^a /77.0	50	30	100
3-ABP	170.0	153.0 ^a /127.0	50	30	100
4-ABP	170.0	153.0 ^a /127.0	50	30	100
1-NA- <i>d</i> ₇	151.0	132.0 ^a /81.0	50	30	100
2-NA- <i>d</i> ₇	151.0	132.0 ^a /81.0	50	30	100
3-ABP- <i>d</i> ₉	179.0	160.0 ^a /136.0	50	30	100
4-ABP- <i>d</i> ₉	179.0	160.0 ^a /136.0	50	30	100

^a The quantitative ion pair.**Fig. 1** Synthesis scheme of magnetic COFs (TpPa-1) material.

characterization (PPMS-9(VSM), Quantum Design, USA). Thermogravimetric analysis (TGA) was measured with TGA IR thermogravimetric analyzer (NETZSCH STA 409 PC, Germany).

2.5. Urine sampling

27 healthy volunteers containing 20 smokers and 7 nonsmokers were recruited into the study. All volunteers were informed

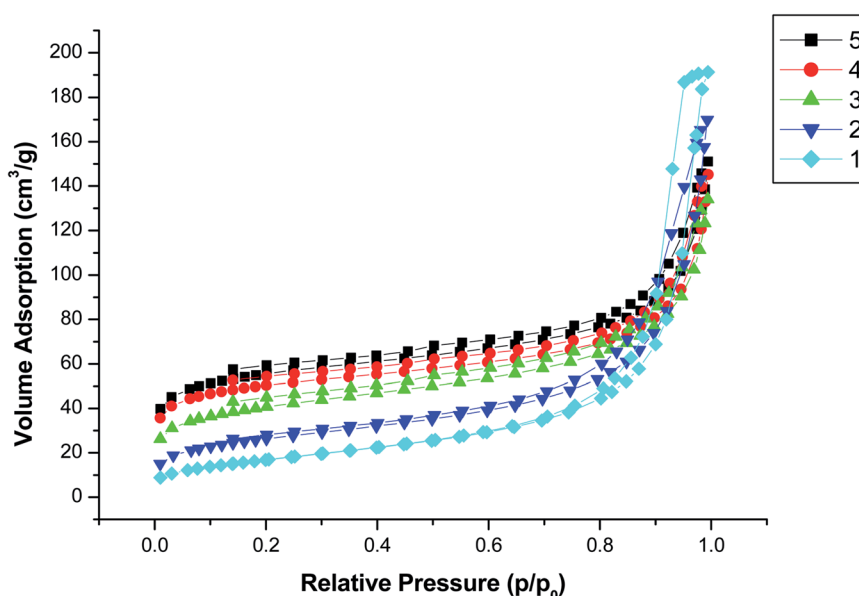
**Fig. 2** Nitrogen adsorption-desorption isotherms of the synthesized materials. (1) Magnetic $\text{NH}_2\text{-Fe}_3\text{O}_4$ material; (2–5) magnetic COFs materials (reaction solvent volume: 2–80 mL, 3–40 mL, 4–30 mL, 5–20 mL).

Table 2 Surface area, pore volume and average pore diameter of the synthesized magnetic materials

Magnetic materials	Solvent volume (mL)	BET surface area (m ² g ⁻¹)	Pore volume (cm ³ g ⁻¹)	Average pore diameter (nm)
NH ₂ -Fe ₃ O ₄	—	62.3	0.29	15.6
Magnetic COFs-2	80	94.3	0.26	8.3
Magnetic COFs-3	40	143.0	0.18	4.4
Magnetic COFs-4	30	174.1	0.18	3.9
Magnetic COFs-5	20	192.1	0.18	3.8

about the aim of this study and freely gave written consent about the donation of urine. Smokers were between 18 and 65 years old, and smoked more than 5 Chinese cigarettes every day for more than 6 months. Urine samples of 24 hours for all persons were collected, and frozen at $-18\text{ }^{\circ}\text{C}$ immediately. Urinary creatinine was determined using an automatic biochemical analyzer (Beckman-coulter SYNCHRON CX9, USA).

2.6. Sample ethical statement

All experiments were performed in accordance with the guidelines “Technical specification of management for field survey in large population-based cohort study (T/CPMA 001-2019)” drafted by Chinese preventive medicine association, and approved by the ethics committee at Zhengzhou University. Informed consents were obtained from human participants of this study.

2.7. Urine sample preparation and MSPE

Urine sample was thawed at room temperature. Before MSPE, sample was treated for acid hydrolysis as follow. 5 mL urine sample was put into 50 mL centrifuge tube, and 1 mL concentrated HCl was added and reacted in $80\text{ }^{\circ}\text{C}$ water bath for 1 h. After cooling in an ice bath, 2.4 mL 5 mol L^{-1} NaOH solution were added to neutralize excess acid and the pH of final urine sample was adjusted to 12–13.

As for MSPE, a certain amount of mixed internal standard solution (1-NA-*d*₇, 2-NA-*d*₇, 3-ABP-*d*₉ and 4-ABP-*d*₉) was added into the treated urine sample. Then, 20 mg magnetic COFs material was added, and the mixture was oscillated for 20 min with vortex apparatus (TALBOYS Advanced multi-tube vortexer, Germany) at room temperature. After extraction of the analytes, an external magnet was utilized to separate the magnetic materials. After urine was discarded, 5 mL water was used to wash the magnetic COFs material, and then 5 mL methanol each time was applied to elute analytes on the magnetic COFs material for three times with 3 min oscillation extraction each. Magnetic COFs material was separated with the help of a magnet. All the elution solution was mixed and dried to 1 mL with a nitrogen blowing concentrator (Caliper Life Sciences Turbovap II, USA) at $50\text{ }^{\circ}\text{C}$, and then 50 μL aqueous ammonia was added and mixed for HPLC-MS/MS analysis.

2.8. Instrument conditions

AA metabolites in urine were determined with an Agilent 1200 HPLC instrument (USA) coupled with an AB SCIEX Triple QUAD 5500 mass spectrometer (AB Sciex Instruments, Germany). A Waters Symmetry ShieldTM RP18 column ($150\text{ mm} \times 2.1\text{ mm}$

i.d., $3.5\text{ }\mu\text{m}$) was chosen for HPLC analysis with the flow rate of $300\text{ }\mu\text{L min}^{-1}$ and the injection volume was 10 μL . The mobile phase A was water with 0.1% formic acid, while B was acetonitrile with 0.1% formic acid. The gradient elution program was as follows: 0–3.0 min, 100% A; 3.1–17.0 min, 78% A and 22% B; 17.1–22.0 min, 100% B; precondition: 5 min.

Mass detection conditions were as follows: ionization mode, positive ESI; ion spray voltage, 5000 V; ion source temperature, $550\text{ }^{\circ}\text{C}$; curtain gas, nitrogen; setting: 30 psi; ion source gas 1 (GS1), setting: 70 psi; ion source gas 2 (GS2), setting: 70 psi. Two ion pairs were chosen as qualitative ion pairs and a quantitative ion pair was used with multiple reaction monitoring (MRM) mode. The parameters of MRM containing precursor ion, production ion, dwell time, collision energy (CE), declustering potential (DP) for four AAs and the internal standards were shown in Table 1.

3. Results and discussion

3.1. Fabrication and characterization of magnetic COFs material

The synthesis of COFs (TpPa-1) material was based on the principle of Schiff-base reaction. Before the synthesis of COFs material, the amino group of magnetic Fe₃O₄ nanoparticles was

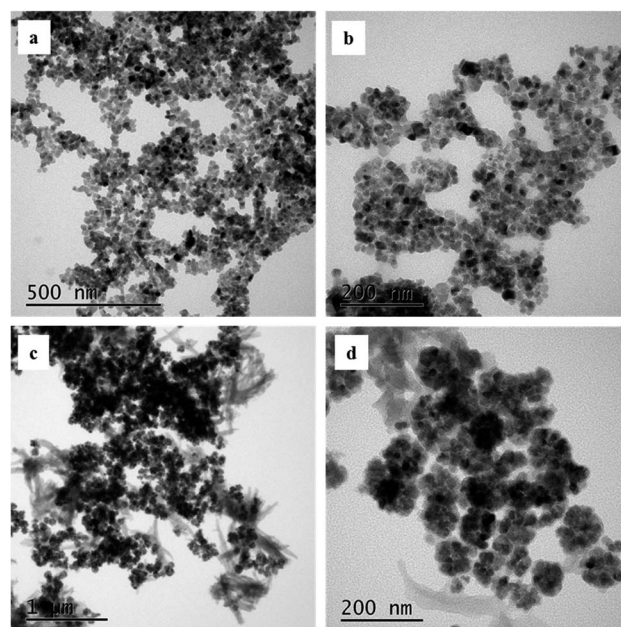


Fig. 3 HRTEM image of synthesized magnetic materials ((a) and (b) magnetic NH₂-Fe₃O₄ nanoparticles; (c) and (d) magnetic COFs material).



reacted with aldehyde group of Tp, which could promote the generation of COFs on the surface of magnetic nanoparticles. The synthesis scheme of magnetic COFs material was shown in Fig. 1. Nitrogen adsorption-desorption isotherm was used to characterize surface area and pore volume of the synthesized magnetic COFs material, which was shown in Fig. 2. The magnetic COFs material exhibited a typical type-I reversible isotherm characteristic of microporous property. However, a sharp rise of adsorption volume at higher relative pressure ($P/P_0 = 1$) for N_2 adsorption-desorption isotherm indicated that large pore formed by particle packing. The BET surface area, pore volume and average pore diameter was shown in Table 2. The influence of temperature, stirring speed, reaction time, reaction solvents and solvent volume on the surface area of the synthesized magnetic COFs materials was investigated in this work. And only reaction solvent volume influenced surface area of the obtained materials obviously. With the decrease of reaction solvent volume, surface area of the obtained materials increased. The magnetic COFs material with the reaction solvent volume of 20 mL showed the highest surface area, which was applied for MSPE of urinary AAs. And the BET surface area was $192.1 \text{ m}^2 \text{ g}^{-1}$, pore volume was $0.18 \text{ cm}^3 \text{ g}^{-1}$, and average pore diameter was 3.8 nm. As for magnetic $\text{NH}_2\text{-Fe}_3\text{O}_4$ nanoparticles, N_2 adsorption-desorption isotherm indicated that large pore existence formed by particle packing. After the information of COFs material on the surface of magnetic $\text{NH}_2\text{-Fe}_3\text{O}_4$

nanoparticles, the obtained magnetic COFs material showed the increased surface area. What's more, the magnetic COFs materials were synthesized with the reaction solvent volume of 20 mL for three times in this work. The BET surface area was 189.3, 192.1, $200.2 \text{ m}^2 \text{ g}^{-1}$, respectively. And their extraction capacity for AAs metabolite in urine was investigated and the results were comparable. Thus, the preparation reproducibility of the magnetic COFs nanoparticles was acceptable. And the prepared magnetic COFs nanoparticles of three times were mixed for the MSPE experiment in the work.

Other structure analysis and characterization was performed for magnetic COFs material with the reaction solvent volume of 20 mL. HRTEM was applied to characterize morphologies of the synthesized magnetic materials as shown in Fig. 3. Magnetic $\text{NH}_2\text{-Fe}_3\text{O}_4$ nanoparticles showed a uniform particle size of about 20 nm. The particle size of magnetic COFs materials (Fig. 3d) was larger than magnetic $\text{NH}_2\text{-Fe}_3\text{O}_4$ nanoparticles (Fig. 3b) due to the formation of COFs on the surface of magnetic nanoparticles. And magnetic COFs material was a complex of COFs@ $\text{NH}_2\text{-Fe}_3\text{O}_4$ nanoparticles and needle shaped COFs materials as shown in Fig. 3c.

FT-IR spectra showed chemical composition and structure information of magnetic nanomaterials. FT-IR spectra of COFs was shown as Fig. 4A. And the characteristic peak at 3500 cm^{-1} corresponding to $-\text{NH}_2$ vibration, the adsorption bands at 1589 cm^{-1} was associated with carboxyl groups, and the peak at

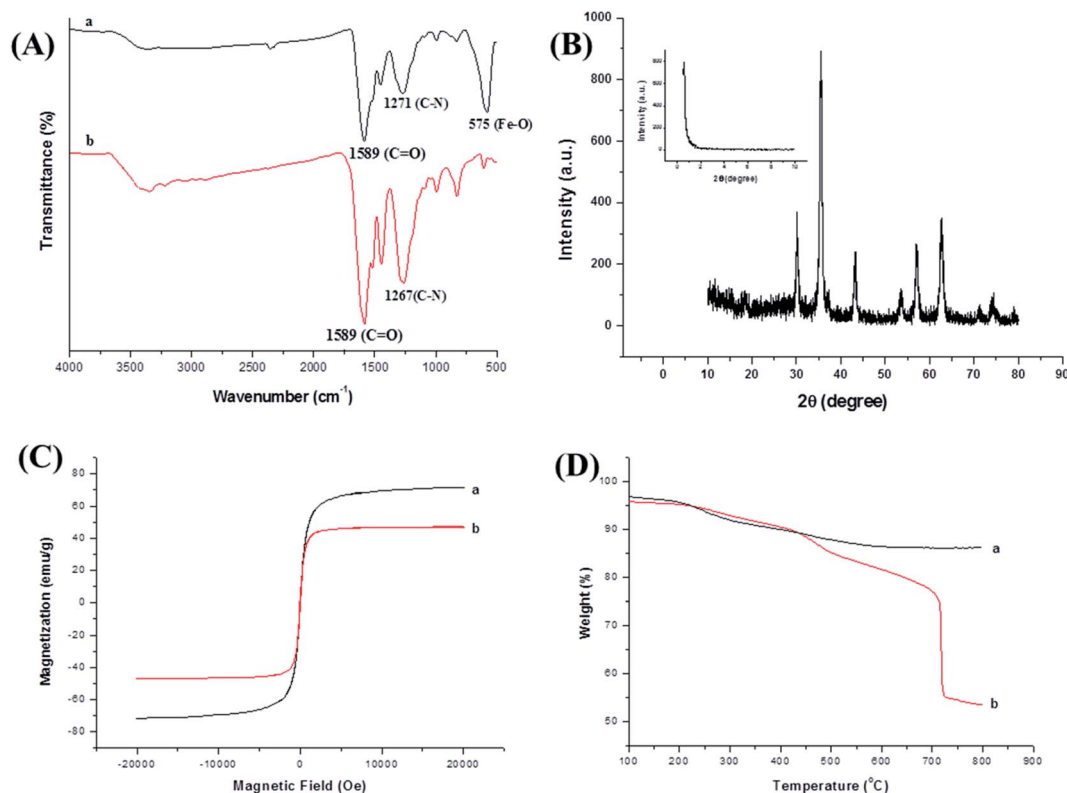


Fig. 4 (A) FT-IR spectra of magnetic COFs (a) and COFs (b); (B) XRD spectra of magnetic COFs, and the inset was SXR spectra; (C) hysteresis loops of magnetic COFs (a) and magnetic $\text{NH}_2\text{-Fe}_3\text{O}_4$ nanoparticles (b); (D) TGA curves of magnetic $\text{NH}_2\text{-Fe}_3\text{O}_4$ nanoparticles (a) and magnetic COFs (b).

1267 cm^{-1} was the characteristic adsorption related to $\text{C}=\text{N}$, which indicated the $\text{C}=\text{N}$ vibration was formed for COFs materials. Compared with COFs material, the FT-IR spectra of magnetic COFs material (Fig. 4A) showed a new characteristic peak at 575 cm^{-1} which was corresponding to the $\text{Fe}-\text{O}-\text{Fe}$ vibration, indicated that COFs material was warped on the magnetic $\text{NH}_2-\text{Fe}_3\text{O}_4$ nanoparticles successfully. XRD spectra were shown in Fig. 4B, which gave the crystalline structure of the obtained magnetic COFs material. The diffraction peaks at 30.1° , 35.4° , 43.2° , 53.7° , 57.1° and 62.9° in the 2θ region of $30-40^\circ$, which can be assigned as (220), (311), (400), (422), (511) and

(440) planes in the magnetic $\text{NH}_2-\text{Fe}_3\text{O}_4$ nanoparticles.²⁵ The diffraction peak at 0.6° in SXRD spectra might be related to the low crystallinity of magnetic COFs material. A magnetic hysteresis curve for magnetic $\text{NH}_2-\text{Fe}_3\text{O}_4$ nanoparticles and magnetic COFs material were shown in Fig. 4C, and the saturation magnetic values were estimated to be 71.8 emu g^{-1} and 46.3 emu g^{-1} , respectively. It was obviously, magnetic COFs material showed lower magnetic property than magnetic $\text{NH}_2-\text{Fe}_3\text{O}_4$ nanoparticles owing to warping with COFs material. However, magnetic COFs material possessed great magnetic responsiveness and could be separated with external magnetic

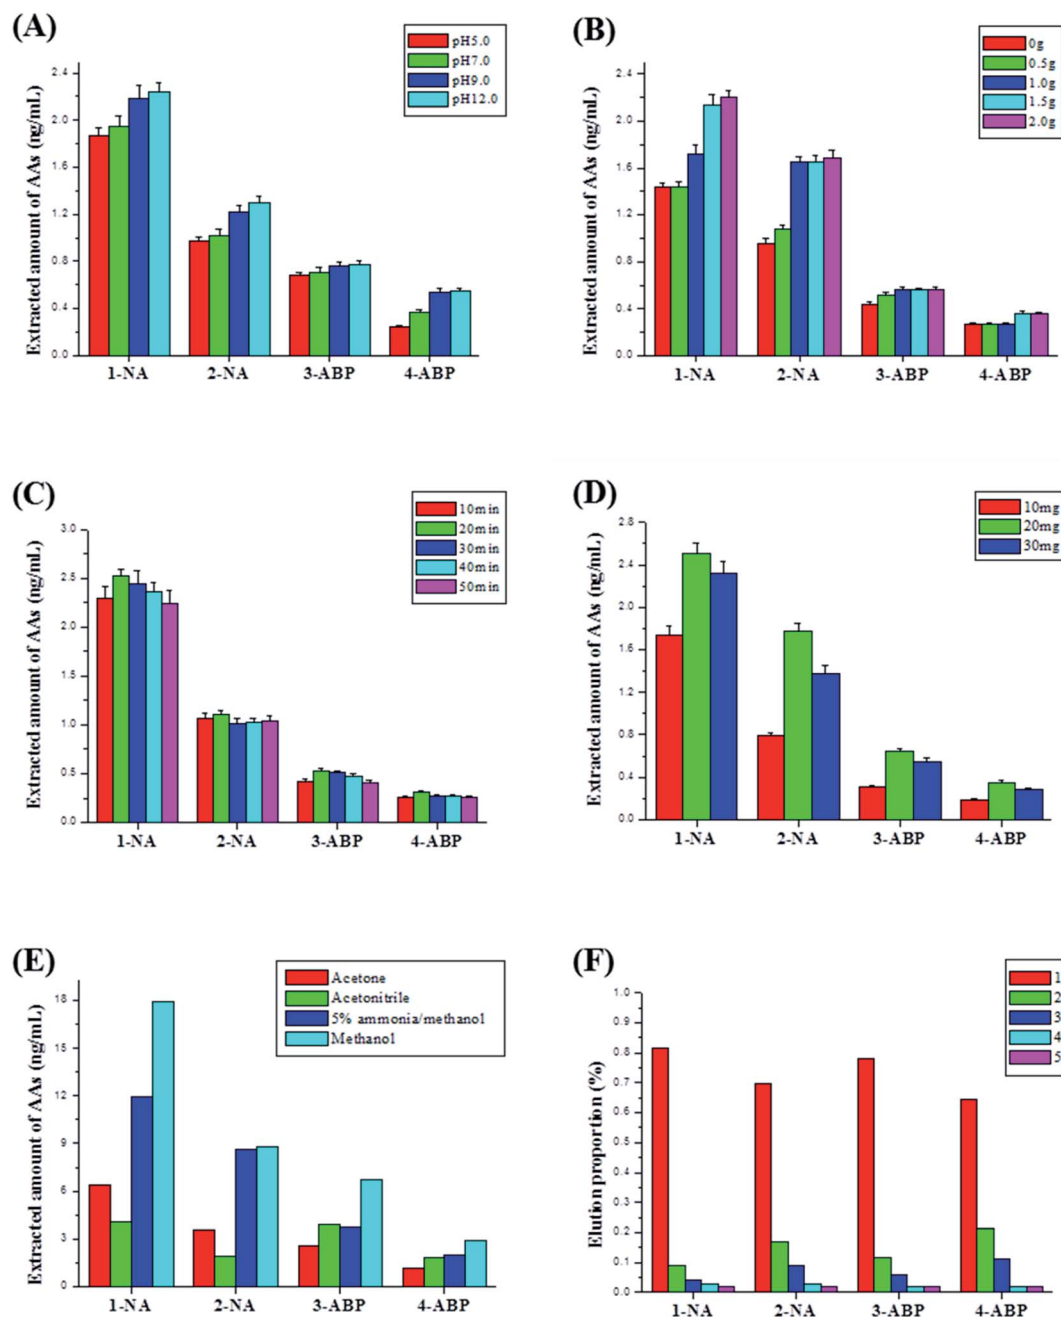


Fig. 5 Effect of MSPE conditions on extraction performance of urinary 4 AAs: (A) sample solution pH, (B) NaCl amount, (C) vortex extraction time, (D) sorbent amount, (E) different elution solvent, (F) elution time. Data in (A)–(D) was average (\pm SD) after three repetition experiments.



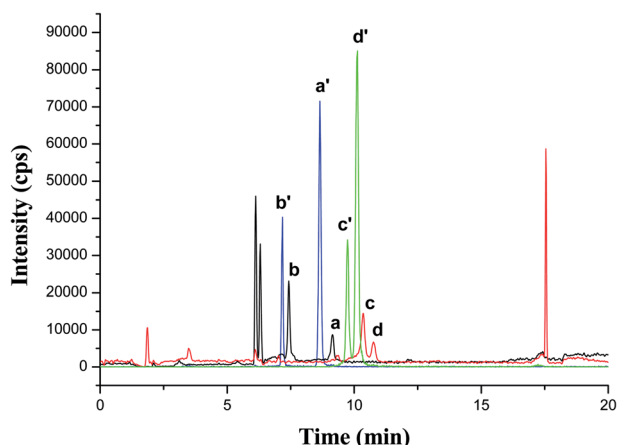


Fig. 6 HPLC-MS/MS-MRM spectra of AAs and their corresponding internal standard in a spiked smoker urine sample. (a) 1-NA; (b) 2-NA; (c) 3-ABP; (d) 4-ABP; (a') 1-NA- d_7 ; (b') 2-NA- d_7 ; (c') 3-ABP- d_9 ; (d') 4-ABP- d_9 .

field. TGA curves were shown in Fig. 4D, which gave the mass ratios of COFs and Fe_3O_4 nanoparticles, and the thermal stability of magnetic COFs material. Magnetic $\text{NH}_2\text{-Fe}_3\text{O}_4$ nanoparticles showed 4.7 wt% loss in the temperature range of 200–300 °C, which was attributed to the weight loss of the absorbed water, and the 5.2 wt% loss in the temperature range of 300–557 °C was due to the loss of amino functional groups on the surface. As for magnetic COFs material, the 6.1 wt% loss in the temperature between 200–430 °C was attributed to the weight of loss of the absorbed water, and 35 wt% loss in the range of 430–730 °C was due to the loss of COFs material. Obviously, the magnetic COFs material had excellent thermal stability under 430 °C.

3.2. Optimization of MSPE conditions

Owing to the lower content of AA metabolites in urine sample, a mixed urine sample spiked with a certain amount of AAs standard solution was used to optimize MSPE conditions and characterize analytical performance of the developed method. To obtain the best extraction performance, some conditions of MSPE were optimized in this work, such as urine solution pH, NaCl amount, vortex extraction time, sorbent amount, different elution solvent and elution time.

Firstly, sample solution pH was investigated. With the increase of sample solution pH, the extracted amount of urinary AAs

increased, and the maximum was obtained at pH about 12.0 (Fig. 5A). The pK_a of 4 AAs (1-NA, 2-NA, 3-ABP and 4-ABP) was 4.21 ± 0.10 , 4.32 ± 0.10 , 4.34 ± 0.10 , 4.26 ± 0.10 , respectively. Thus, they were almost completely molecular state when the solution pH of 12.0–13.0. What's more, the synthesized magnetic COFs (TpPa-1) material possessed imine groups in the framework, and showed molecular state in higher pH solution also. At higher pH solution (*i.e.* pH 12.0–13.0), AAs compounds could be easily adsorbed on the magnetic COFs materials due to π - π stacking. Thus, after acid hydrolysis, urine was adjusted to about pH 12.0–13.0 for MSPE in this work. To further improve extraction efficiency, a certain amount of NaCl was added into the treated urine for salting-out effect. As shown in Fig. 5B, with the increase of NaCl amount, the extracted amount of AAs enhanced until the addition amount of 2.0 g. When continuing to add NaCl, it could not be dissolved and a NaCl saturated solution was obtained. Thus, the amount of NaCl added was 2.0 g. Influence of vortex extraction time and magnetic absorbent amount used were studied also. As shown in Fig. 5C and D, the maximum extracted amount of AAs could be obtained after 20 min vortex extraction with 20 mg the synthesized magnetic COFs material.

After vortex extraction, different solvent was used to elute, such as acetone, acetonitrile, 5% ammonia/methanol and methanol. As shown in Fig. 5E, the maximum extracted amount of AAs was obtained with methanol as elution solvent. The extracted amount of AAs after methanol elution was higher than that for 5% ammonia/methanol, which indicated there was mainly π - π stacking, not electrostatic interaction between AAs and magnetic COFs (TpPa-1) material. And as shown in Fig. 5F, after elution with 5 mL methanol, 80% 1-NA, 60% 2-NA, 70% 3-ABP and 60% 4-ABP was eluted from magnetic COFs. And after 3 times elution, over 95% of all AAs were eluted. Thus, 5 mL methanol each for three times was applied to elute AAs on magnetic COFs sorbent.

A spiked smoker urine sample was analyzed with HPLC-MS/MS technique after MSPE under the optimized conditions. As shown in Fig. 6, both 4 AAs and their corresponding isotope internal standard showed well-defined peaks, which could satisfy quantitative analysis.

3.3. Analytical parameters

AAs standard working solution was prepared with 5% ammonia/methanol, which showed a well-defined chromatographic peak in HPLC-MS/MS, while standard working solution prepared with methanol gave a poor peak. A 5-point calibration

Table 3 Linear concentration range, calibration curve in solvent and urine matrix, LOD and LOQ of the developed method

Compounds	Linear concentration range (ng mL ⁻¹)	Calibration curve in solvent	Calibration curve in urine matrix	Slope ratio	LOD (ng mL ⁻¹)	LOQ (ng mL ⁻¹)
1-NA	0.5–25	$y = 0.102x - 0.014$ ($r = 0.9999$)	$y = 0.102x - 0.026$ ($r = 0.9996$)	1.00	0.07	0.22
2-NA	0.25–12.5	$y = 0.259x - 0.0086$ ($r = 1$)	$y = 0.268x - 0.0080$ ($r = 0.9997$)	0.97	0.03	0.09
3-ABP	0.10–5.0	$y = 0.276x + 0.00049$ ($r = 0.9998$)	$y = 0.274x + 0.051$ ($r = 0.9994$)	1.01	0.01	0.04
4-ABP	0.05–2.5	$y = 0.0558x + 0.00036$ ($r = 0.9996$)	$y = 0.0507x + 0.035$ ($r = 0.9896$)	1.10	0.01	0.04



Table 4 Recovery, inter-day and intra-day precision of the developed method

Compounds	Spiked level	Recovery (%)	Intra-day precision ($n = 6$, %)	Inter-day precision ($n = 5$, %)
1-NA	Low	81.9–95.2	4.5	9.8
	Mid	100–105		
	High	95.7–101		
2-NA	Low	87.8–92.8	4.6	8.3
	Mid	89.9–102		
	High	97.8–101		
3-ABP	Low	102–112	5.6	9.1
	Mid	101–120		
	High	101–107		
4-ABP	Low	102–112	5.8	9.9
	Mid	88.3–117		
	High	89.8–93.9		

curve was carried out by internal standard method. The concentration of 1-NA- d_7 , 2-NA- d_7 , 3-ABP- d_9 and 4-ABP- d_9 for each working solutions was 20 ng mL⁻¹, 15 ng mL⁻¹, 7 ng mL⁻¹, 16 ng mL⁻¹, respectively. Another calibration curve was prepared with urine matrix, which was calibrated by spiking a series of AAs standard solution in nonsmokers' urine extracts after MSPE based on magnetic COFs material. And the final concentration range was the same as that of calibration curve in solvent. The series of standard working solution prepared in solvent and urine matrix were analyzed using HPLC-MS/MS. And the linear concentration range of AAs and linear equation was shown in Table 3. According to the linear correlation coefficient (r), the linearity was good for calibration curves for both solvent and urine matrix ($r > 0.99$). What's more, as shown in Table 3, the slope ratios of two linear equations for four AAs are 1.00, 0.97, 1.01, 1.10, respectively. It indicated matrix effect was decreased significantly, which was attributed to that respective isotope internal standards of AAs were used, and urine sample was purified effectively with MSPE technique based on magnetic COFs material. Thus, the calibration curve in solvent could replace the calibration curve in urine matrix, and could be used for urine samples analysis.

In addition, the lowest concentration standard working solution prepared in urine matrix was determined in HPLC-MS/MS for ten replicates. Limit of detection (LOD) and limit of quantification (LOQ) were obtained from three and ten times of the standard deviation of these determinations. As shown in Table 3, LODs and LOQs of four AAs ranged from 0.01 to 0.07 ng mL⁻¹ and 0.04 to 0.22 ng mL⁻¹, respectively. Compared with previous work, the LODs of this work were higher than those of four AAs metabolite in urine using a MIPs-SPE coupled with HPLC-MS/MS method in our previous work⁹ (*i.e.* 1.5–5 ng L⁻¹). It was mainly because that the LODs in this work was conducted with the lowest concentration working solution prepared in urine matrix, but the LODs in ref. 9 was obtained with the lowest concentration working solution in solvent. However, the LOQs of AAs in this work were lower than the lowest concentration of calibration curve, which satisfied the requirement of quantitative analysis.

In order to assess the recovery, a smoker urine sample with spiking standard solution of AAs in three different concentration levels was analyzed. Each concentration level was performed with three replicate measurements. As is shown in Table 4, higher recoveries of 1-NA, 2-NA, 3-ABP, 4-ABP were obtained, which are in the range of 81.9–105%, 87.8–102%, 101–120%, 88.3–117%, respectively. Intra-day and inter-day precisions were

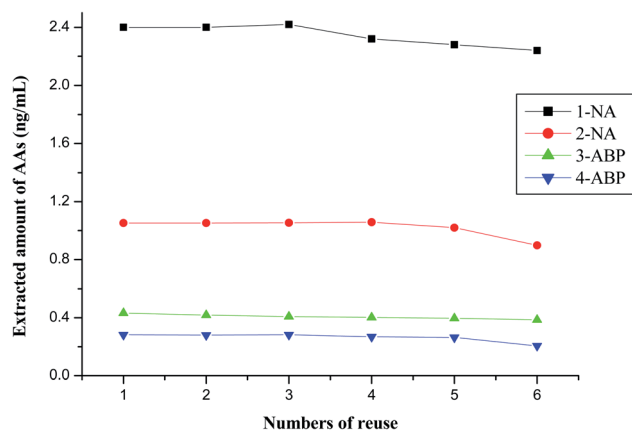


Fig. 7 Extracted amount of AAs after several times reuse.

Table 5 Statistical result of 4 AA metabolites content in smoker and nonsmoker urine samples

		AA metabolites content (pg mg ⁻¹ creatinine)			
	Compounds	Maximum	Minimum	Median	Average
Smoker	1-NA	492	9	169.73	189.60
	2-NA	1463	25	281.99	416.21
	3-ABP	720	0	103.80	172.87
	4-ABP	2184	14	264.82	419.27
Nonsmoker	1-NA	184	0	20.37	39.56
	2-NA	282	0	45.17	66.22
	3-ABP	0	0	0	0
	4-ABP	48	0	9.87	15.99



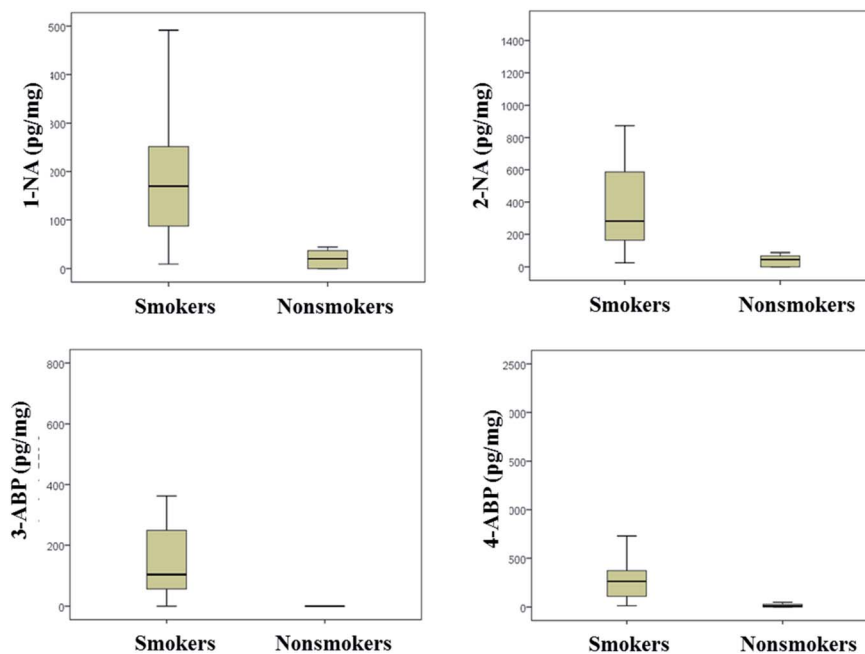


Fig. 8 Average and variation range of AA metabolites in smoker and nonsmoker urine samples.

investigated using a spiked urine sample (Table 4). The urine sample was analyzed 6 times on the same day to investigate the intra-day precision, and the RSDs were less than 5.8%. And the urine sample was analyzed on 5 different days to obtain the inter-day precision, and the RSDs were less than 9.9%.

3.4. Recycle performance

The recycle performance of magnetic COFs material was investigated also. As shown in Fig. 7, the extracted amount of 4 AAs maintained over 90% after 5 times reuse. However, the extracted amount of AAs was less than 90% at 6 times reuse. Thus, the synthesized magnetic COFs material could be recycled as sorbent in MSPE process for at least 5 times.

Owing to the ultra-low content of AA metabolites in urine, a MIPs-SPE was chosen to purify urine for AA metabolites analysis,⁹ while a mixed type cation exchange SPE cartridge was suitable for purifying cigarette smoke sample¹³ nor urine sample⁹ for AAs analysis as shown in our previous work.^{9,13} Magnetic COFs material prepared in this work also could purify urine matrix and achieve the analysis of AA metabolites. However, compared with commercial SPE columns used in previous works which applied HPLC-MS/MS technique,^{9,13} the magnetic COFs material and MSPE showed some advantages. For example, the magnetic COFs material could recycle, which was more economical. And the sample pretreatment with MSPE technique was simple and practicable.

3.5. Human urine samples analysis

The developed method was applied to determine 4 AA metabolites in 27 urine samples collected from 20 smokers and 7 nonsmokers. And the result was calibrated with urinary creatinine and analysis of variance was applied for data processing.

Table 5 and Fig. 8 showed the maximum, the minimum, the median, the average and variation range of 4 AA metabolites content in smoker and nonsmoker urine. It was obviously, all 4 AA metabolites content in smoker urine sample was higher than that for nonsmoker. And the *P* value between smoker and nonsmoker for 1-NA, 2-NA, 3-ABP and 4-ABP was 0.0009, 0.0006, 0.0008, and 0.0030 (*i.e.* $p < 0.01$), respectively, which indicated there was significant difference between the 4 AA metabolites content in smoker and nonsmoker urine. Thus, urinary AA metabolites could be as an exposure biomarker for cigarette smoke.

4. Conclusion

A magnetic COFs (TpPa-1) material was synthesized and characterized in this work. The magnetic COFs material based MSPE technique was developed for the determination of AA metabolites (*i.e.* 1-NA, 2-NA, 3-ABP and 4-ABP) in urine with HPLC-MS/MS analysis. Under the optimum conditions of MSPE, the analytical performance of the developed method was characterized also. Calibration curves in solvent and urine matrix were conducted, and their slope was near. It indicated that matrix effect was decreased significantly attributing to the effective purification with MSPE based on magnetic COFs material. LODs and LOQs of four AAs ranged from 0.01 to 0.07 ng mL⁻¹ and 0.04 to 0.22 ng mL⁻¹, respectively. As for recovery, 1-NA, 2-NA, 3-ABP, 4-ABP were in the range of 81.9–105%, 87.8–102%, 101–120%, 88.3–117%, respectively. The intra-day and inter-day precisions were good also with RSDs of less than 5.8% and 9.9%, respectively. In addition, the synthesized magnetic COFs material could be recycled as sorbent in MSPE process for at least 5 times. The developed method was applied in the determination of four AAs in urine samples of smokers and

nonsmokers. AA metabolites contents in smoker urine samples were higher than those for nonsmoker. And there were significant difference between smoker and nonsmoker urine ($p < 0.01$). Thus, urinary AA metabolites could be as an exposure biomarker for cigarette smoke.

Conflicts of interest

There are no conflicts to declare.

Acknowledgements

The authors appreciate the support from the National Natural Science Foundation of China (No. 31901768).

References

- Food and Drug Administration, *Harmful and Potentially Harmful Constituents in Tobacco Products and Tobacco Smoke; Established List*, Docket No. FDA-2012-N-0143.
- IARC Monographs on the Evaluation of Carcinogenic Risks to Humans, IARC, 2013, <http://www.monographs.iarc.fr/ENG/Classification/index.php>, accessed 30 July 2013.
- IARC Monographs on the evaluation of the carcinogenic risk of chemicals to humans. *Chemicals industrial processes and industries associated with cancer in humans*, Lyon, 1982.
- G. Grimmer, G. Dettbarn, A. Seidel and J. Jacob, *Sci. Total Environ.*, 2000, **247**, 81–90.
- K. Riedel, G. Scherer, J. Engl, H. W. Hagedorn and A. R. Tricker, *J. Anal. Toxicol.*, 2006, **30**, 187–195.
- P. Kämpfer, S. Crettaz, S. Nussbaumer, M. Scherer, S. Krepich and O. Deflorin, *J. Chromatogr. A*, 2019, **1592**, 71–81.
- B. J. Brüsweiler and C. Merlot, *Regul. Toxicol. Pharmacol.*, 2017, **88**, 214–226.
- T. Carreon, M. J. Hein, K. W. Hanley, S. M. Viet and A. M. Ruder, *Occup. Environ. Med.*, 2014, **71**, 175–182.
- J. J. Yu, S. Wang, G. Zhao, B. Wang, L. Ding, X. B. Zhang, J. P. Xie and F. W. Xie, *J. Chromatogr. B: Anal. Technol. Biomed. Life Sci.*, 2014, **958**, 130–135.
- J. J. Niu, X. L. Zhao, Y. Y. Jin, G. T. Yang, Z. H. Li, J. J. Wang, R. Q. Zhao and Z. Y. Li, *J. Chromatogr. A*, 2018, **1555**, 37–44.
- S. Mazumder, R. A. Ahamed, E. McGahee, L. Q. Wang and T. H. Seyler, *J. Anal. Toxicol.*, 2019, **43**, 25–35.
- S. Saha, R. Mistri and B. C. Ray, *J. Chromatogr. A*, 2009, **1216**, 3059–3063.
- F. W. Xie, J. J. Yu, S. Wang, G. Zhao, Q. L. Xia, X. B. Zhang and S. S. Zhang, *Talanta*, 2013, **115**, 435–441.
- A. P. Cote, A. I. Benin, N. W. Ockwig, M. O'Keeffe, A. J. Matzger and O. M. Yaghi, *Science*, 2005, **310**, 1166–1170.
- X. Feng, X. Ding and D. Jiang, *Chem. Soc. Rev.*, 2012, **41**, 6010–6022.
- S. Y. Ding and W. Wang, *Chem. Soc. Rev.*, 2013, **42**, 548–568.
- A. P. Cote, H. M. El-Kaderi, H. Furukawa, J. R. Hunt and O. M. Yaghi, *J. Am. Chem. Soc.*, 2007, **129**, 12914–12915.
- Y. Liu, Y. Ma, Y. Zhao, X. Sun, F. Gándara, H. Furukawa, Z. Liu, H. Zhu, C. Zhu and K. Suenaga, *Science*, 2016, **351**, 365–369.
- N. Huang, X. Chen, R. Krishna and D. Jiang, *Angew. Chem., Int. Ed.*, 2015, **54**, 2986–2990.
- S. Wan, J. Guo, J. Kim, H. Ihee and D. Jiang, *Angew. Chem., Int. Ed.*, 2009, **121**, 5547–5550.
- R. Wang and Z. L. Chen, *Microchim. Acta*, 2017, **184**, 3867–3874.
- L. Chen, Y. T. He, Z. X. Lei, C. L. Gao, Q. Xie, P. Tong and Z. Lin, *Talanta*, 2018, **181**, 296–304.
- S. J. He, T. Zeng, S. H. Wang, H. Y. Niu and Y. Q. Cai, *ACS Appl. Mater. Interfaces*, 2017, **9**, 2959–2965.
- Y. H. Yan, Y. J. Lu, B. C. Wang, Y. Q. Gao, L. L. Zhao, H. Z. Liang and D. P. Wu, *ACS Appl. Mater. Interfaces*, 2018, **10**, 26539–26545.
- C. H. Gao, G. Lin, Z. X. Lei, Q. Zheng, J. S. Lin and Z. Lin, *J. Mater. Chem. B*, 2017, **5**, 7496–7503.
- W. F. Zhang, Y. H. Zhang, G. R. Zhang, J. Y. Liu, W. D. Zhao, W. J. Zhang, K. Hu, F. W. Xie and S. S. Zhang, *Analyst*, 2019, **144**, 5829–5841.
- W. F. Zhang, C. Lan, H. M. Zhang, Y. H. Zhang, W. J. Zhang, W. D. Zhao, C. Johnson, K. Hu, F. W. Xie and S. S. Zhang, *J. Agric. Food Chem.*, 2019, **67**, 3733–3743.
- Y. H. Zhang, Y. Y. Song, J. Wu, R. J. Li, D. Hu, Z. A. Lin and Z. W. Cai, *Chem. Commun.*, 2019, **55**, 3745–3748.
- L. Y. Wang, J. Bao, L. Wang, F. Zhang and Y. D. Li, *Chem.–Eur. J.*, 2006, **12**, 6341–6347.
- J. Tan, S. Namuangruk, W. F. Kong, N. Kungwan, J. Guo and C. C. Wang, *Angew. Chem., Int. Ed.*, 2016, **55**, 1–7.
- S. J. He, T. Zeng, S. H. Wang, H. Y. Niu and Y. Q. Cai, *ACS Appl. Mater. Interfaces*, 2017, **9**, 2959–2965.

