


 Cite this: *RSC Adv.*, 2023, 13, 24319

## Correction: Indocyanine-green-loaded microbubbles for localization of sentinel lymph node using near-infrared fluorescence/ultrasound imaging: a feasibility study

 Long Wang,<sup>b</sup> Yihe Hu,<sup>b</sup> Qinghai Peng,<sup>a</sup> Jiawei Zhou,<sup>a</sup> Qichang Zhou,<sup>a</sup> Senbo An<sup>b</sup> and Chengcheng Niu<sup>\*a</sup>

DOI: 10.1039/d3ra90075d

[rsc.li/rsc-advances](https://rsc.li/rsc-advances)

 Correction for 'Indocyanine-green-loaded microbubbles for localization of sentinel lymph node using near-infrared fluorescence/ultrasound imaging: a feasibility study' by Long Wang *et al.*, *RSC Adv.*, 2016, 6, 50513–50520, <https://doi.org/10.1039/C5RA26814A>.

The authors regret an error in the original article whereby identical images were presented in Fig. 5a for ICG-PLGA (2 h) and in Fig. 5b for ICG (0 h) and ICG-PLGA (2 h). The correct Fig. 5 is provided here.

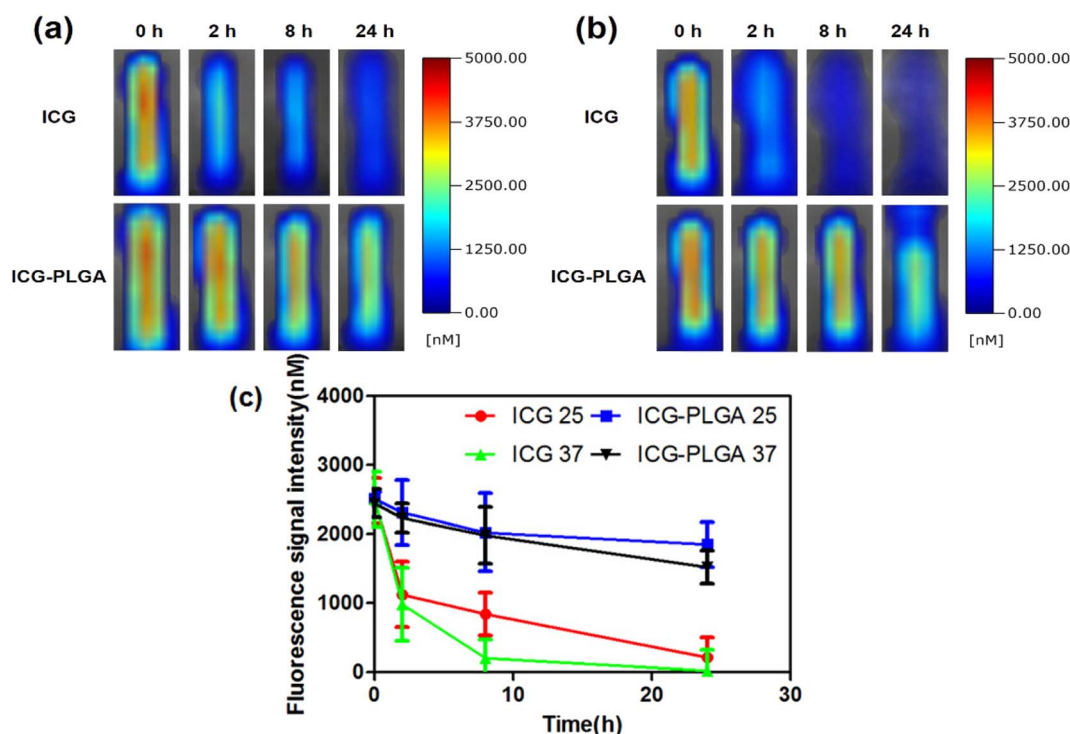


Fig. 5 Comparison of the fluorescence stability of ICG and ICG-PLGA microbubbles. Using the NIR fluorescence images, ICG-PLGA microbubbles were compared to ICG in water at (a) 25 °C and (b) 37 °C within a time of 24 hours. Plot for fluorescence stability of the ICG and ICG-PLGA microbubbles over time (24 hours) when incubated in water at 25 °C and 37 °C (c).

The Royal Society of Chemistry apologises for these errors and any consequent inconvenience to authors and readers.

<sup>a</sup>Department of Ultrasound, The Second Xiangya Hospital, Central South University, Changsha, 410000, P. R. China. E-mail: [cici204675@163.com](mailto:cici204675@163.com); Tel: +86 85292140

<sup>b</sup>Department of Orthopedics, Xiangya Hospital, Central South University, Changsha, 410000, P. R. China

