


 Cite this: *Sens. Diagn.*, 2023, 2, 36

 Received 15th September 2022,
 Accepted 4th October 2022

DOI: 10.1039/d2sd00165a

rsc.li/sensors

Research progress of electrode materials for non-enzymatic glucose electrochemical sensors

 Jianjun Liu,^{*a} Jijun Shen,^b Shengchao Ji,^a Qingyang Zhang^a and Wei Zhao^c

Glucose biosensors are mainly divided into two types. Traditional enzymatic glucose sensors with high sensitivity and selectivity were developed and used early; however, they are sensitive to temperature and pH and come at a high cost. In contrast, non-enzymatic glucose sensors have been widely studied because of their stability and economy. Their research directions mainly focus on improving the detection ability and immediacy. Under these research directions, different electrode sensitive materials have been continuously developed and studied. This article reviewed the research progress of non-enzymatic glucose electrochemical sensor sensitive materials in the past five years. We also introduced the basic principles of electrochemical detection, various electrode sensitive materials and the development direction of non-enzymatic glucose sensors.

1 Introduction

The commonly used methods of glucose detection are high performance liquid chromatography,¹ spectrophotometry² and a glucose biosensor method.³ Most of the commercially available glucose detection devices are based on biological enzymes, and they are the most researched and commercialized biosensors in the field of biosensing.^{4,5} In 1964, Lyons *et al.*⁶ proposed the use of biological enzymes as an electrode to detect glucose, which laid a theoretical foundation for the development of bio-enzyme glucose detection. The enzymatic glucose sensor needs the participation of oxygen in the process of catalyzing glucose, and the detection result is greatly affected by oxygen concentration. The electrode active material of the non enzymatic glucose electrochemical sensor is an inorganic material, which gets rid of some limitations of biological enzymes. Therefore, compared with the enzymatic glucose electrochemical sensor, the non-enzymatic glucose electrochemical sensor has the following advantages: firstly, as active substances, inorganic materials have better chemical stability and thermal stability than biological enzymes. Secondly, the synthesis method for inorganic materials is relatively simple, and the cost is low. Finally, inorganic materials have a relatively long storage time and better reproducibility.⁷

2 Detection mechanisms of non-enzymatic glucose sensors

The most important factor in the response of non-enzymatic glucose sensors to glucose is the electrode-sensitive material on the electrode surface. The reaction mechanism between electrode-sensitive materials and glucose can be explained by the following two models. The first is the activated chemisorption model proposed by Pletcher⁸ in 1984, and the second is the initial hydrous oxide/atomic medium model (IHOAM) proposed by Burke⁹ in 1994.

As shown in Fig. 1, Pletcher assumes that glucose molecules are first adsorbed on the electrode surface during the catalytic oxidation of glucose. Due to the unpaired d-electrons and unfilled d-orbitals of the transition metal atoms on the surface of the electrode, they are susceptible to redox reactions with the adsorbed glucose molecules. The C–H bond on the hemiacetal carbon of the glucose molecule breaks and combines rapidly with the electrode surface to form a chemical bond.

The activated chemisorption model only explains the adsorption process on the electrode surface but does not consider the oxidation of hydroxyl radicals. Burke discovered

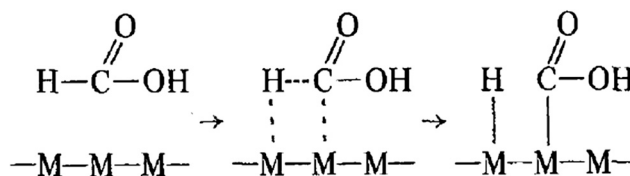


Fig. 1 Mechanism of the activated chemisorption model⁸ (M: metal atom, C: hemiacetal carbon atom).

^a Liaoning Dongke Electric Power Co., Ltd, Shenyang, 110000, China.

E-mail: 1456322196@qq.com

^b State Grid Liaoning Electric Power Co., Ltd., State Grid Liaoning Electric Power Research Institute, Shenyang, 110000, China

^c Xi'an Thermal Power Research Institute Co., Ltd, Xi'an, 710054, China



that the active atoms on the electrode surface have low lattice coordination values and lattice stability, and the polycrystalline surface of the discontinuous region is directly exposed to the solution, which has higher reactivity and is prone to pre-monolayer oxidation. Therefore, he proposed an initial aqueous oxide atomic medium model in 1994, as shown in Fig. 2, the active metal atom on the surface of the electrode undergoes pre-monolayer oxidation to form an initial hydrated oxide layer. The activation layer acts as a medium and an inhibitor in the oxidation and reduction processes to oxidize glucose to gluconolactone.

3 Structure of nanomaterials for glucose detection

There are many structures of nanomaterials, such as hollow sphere,¹⁰ slice type,¹¹ rod shape,¹² flower shape¹³ *etc.* The catalytic effect of different nanostructured electrode materials on glucose is mainly reflected in two aspects: the number of exposed active sites and the size of a surface area. Glucose oxidation involves surface adsorption sites and hydroxyl radicals, both of which can promote the electrochemical oxidation of glucose. Nanoparticles, nanowires and other structures can expose more active sites, which can enhance the electrocatalysis of the electrode surface; in addition, the rough surface can increase the electrochemically active area, participate in more electrochemical reactions, and generate a larger response current. Wei¹⁴ believed that electrode materials with complex hollow architectures, large specific surface area, and porosity, as well as more inner cavities, are widely employed for high-performance supercapacitors. They prepared a complex nickel cobalt manganese sulfide yolk-shell hollow sphere and proved their potential application in high-performance electrochemical energy storage (Fig. 3).

The roughness of the electrode material can be used to increase the Faraday current of slow reaction, Park *et al.*¹⁵ used this principle to construct an electrode material with a mesoporous structure on the surface of a platinum electrode and used it for the detection of glucose. Park *et al.*¹⁶ studied the electrochemical behavior of a 3D-npPt membrane in the electrocatalytic oxidation, O₂ reduction and H₂O₂ reduction of glucose. By comparing the glucose oxidation process on

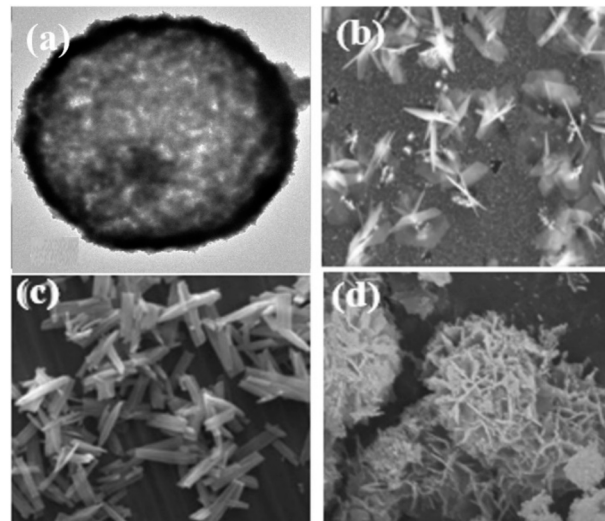


Fig. 3 (a) SEM image of the CuC₂O₄ hollow sphere.¹⁰ (b) SEM image of the Cu₂O/AuCu/Cu sheet.¹¹ (c) SEM image of the NiCo₂S₄ nanorods.¹² (d) SEM image of flower-like NiO.¹³

3D-npPt and 1D nanoporous Pt (1D-npPt), they found that the overall electrode activity of 3D-npPt was significantly higher than that of 1D-npPt, and the high catalytic activity is attributed to the 3D structure of 3D-npPt, which increases the active area of the electrode and reduces the pore resistance.

4 Electrode sensitive material for non-enzymatic glucose sensors

4.1 Precious metal-based non-enzymatic glucose sensors

Pt has high catalytic activity for small molecular substances, it will not dissolve even in a strong acid, strong alkali and high concentration salt medium. The surface of Pt easily adsorbs small molecules due to insufficient d orbital loading and further redox reaction with adsorbate at a certain potential. Therefore, it is considered to be a highly efficient electrocatalyst and is widely used in fuel cells, water decomposition and glucose detection. Au can also react with glucose to generate redox current under neutral or basic conditions, but the effect is not as good as Pt.¹⁷

As shown in Fig. 4, Shim *et al.*¹⁸ incorporated Au into Au@Pt NPs to obtain Au@Pt/Au NPs by an acousto chemical method and a potential step method. The Au core and the Pt shell can increase the selectivity and sensitivity to glucose by synergistic catalytic effects, and the bimetallic core-shell structure prevents metal passivation. Electrochemical performance tests showed that the electrode has a good linear relationship to glucose in the wide linear range of 0.5–10 μM and 100–10 000 μM, and the detection limit is 445 nM. Table 1 summarizes the glucose sensors based on Au and Pt in recent years and shows the key performance parameters such as sensitivity, detection range and minimum detection limit.

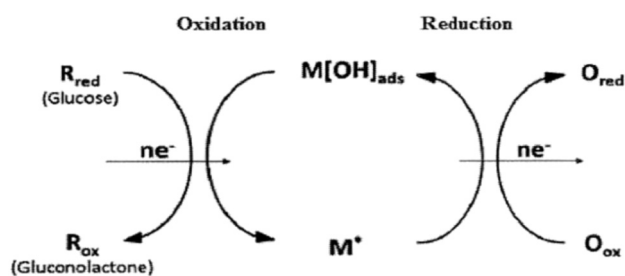


Fig. 2 Mechanism of IHOAM.⁹



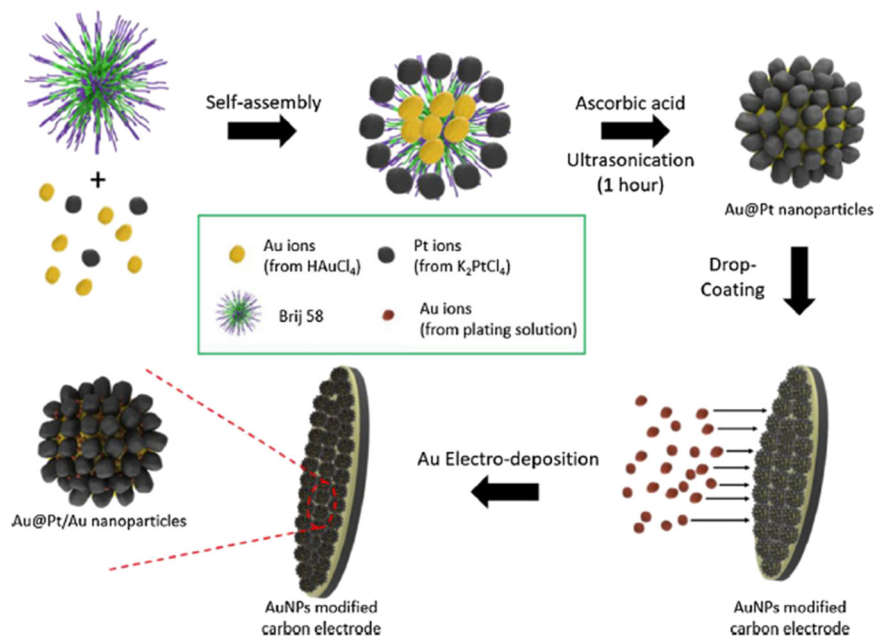


Fig. 4 Schematic illustration of the synthesis of Au@Pt/Au NPs.¹⁸

4.2 Non-enzymatic glucose sensors based on transition metals and their compounds

Transition metal sensing materials have the characteristics of rapid response, high sensitivity, good stability and low cost, which showed unique advantages in the field of glucose enzyme free electrochemical sensors.²² In the process of catalytic oxidation of glucose, transition metal-based electrode sensitive materials mainly involve redox reactions between transition metal compounds with different valence states.²³ The hemiacetal carbon atom of the glucose molecule is dehydrogenated on the surface of the electrode and then combined with the active site adjacent to the surface of the electrode. The dehydrogenated free radical intermediate is further oxidized to gluconolactone and finally oxidized to gluconolactone by hydrolysis. During the reaction, the transition peak of the transition metal compound coincides with the oxidation peak of glucose, which proves that the transition metal acts as a reactive center to participate in the catalytic oxidation process of glucose.²⁴ Metal and metal compound electrodes based on Cu, Co, and Ni have become research hotspots due to their good catalytic properties among many transition metal materials.

4.2.1 Non-enzymatic glucose sensors based on copper and its compounds. Copper is a very promising metal material

with good electrical conductivity and abundant reserves on earth. Various forms of Cu-based glucose sensors have been developed, such as Cu,²⁵ Cu₂O,²⁶ CuO,²⁷ and CuS.²⁸ The oxidation peak range of Cu based materials is wider than that of many catalysts, about 0.3 to 0.5 V (relative to Ag/AgCl). However, the oxidation peak of Cu(II) contains a high background current, and it is difficult to distinguish when the intensity of the oxidation peak is weak.

Liu *et al.*²⁹ synthesized a copper oxide nano-array (CuO NWA) on copper foam (CF) (Fig. 5); the nano-array on the CF increases the specific surface area and the number of active sites, and it also increases the electron transport rate and enhances the electrocatalytic performance. The CuO NWA electrode exhibits an extremely high sensitivity (32 330 $\mu\text{A mM}^{-1} \text{cm}^{-2}$) to glucose in the concentration range of 10 to 500 μM and an ultra-low detection limit (20 nM). It has a lower relative standard deviation when the sensor is used to detect glucose in iced black tea. Table 2 summarizes the Cu-based glucose sensors in the past three years and shows the key performance parameters in detail.

4.2.2 Non-enzymatic glucose sensors based on cobalt and its compounds. Cobalt-based metal compounds have been widely studied as catalysts in the field of glucose sensor sensitive materials.³⁴ Cobalt oxide has three polymorphic substances: CoO, Co₂O₃ and Co₃O₄. Compared with the other

Table 1 List of Au-based and Pt-based electrochemical non-enzymatic glucose sensors

Electrode materials	Sensitivity ($\mu\text{A mM}^{-1} \text{cm}^{-2}$)	Linear range (μM)	LOD (μM)	Operation potential (V)	Chemical environment	Ref.
Au foam	—	0.5–12 000	0.14	0.10	0.3 M NaOH	19
Au/ZnO	4416	~15 000	0.12	0.80	0.1 M PBS (pH = 7.0)	20
Pt/Au	—	0.5–10, 10–10 000	0.45	0.35	0.1 M PBS (pH = 7.4)	18
Ag@Ni-MOF	160.08	5–500	5	0.50	0.1 M NaOH	21




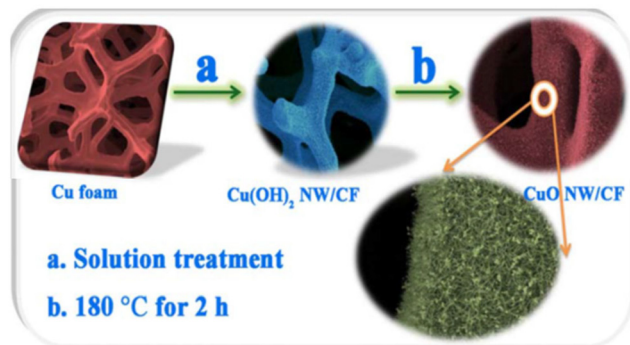


Fig. 5 Fabrication procedure of CuO NWA/CF.²⁹

two polymorphic materials, Co_3O_4 is cheap and environmentally friendly and has high electrical conductivity and electrocatalytic properties.³⁵ Cobalt exists in various forms in an alkaline solution, and there are many redox peaks in the cyclic voltammogram of cobalt involving Co (0)/Co(II), Co(II)/Co(III), and Co(III)/Co(IV) transitions. Studies have found that most catalytic oxidation reactions for glucose are carried out by Co(III)/Co(IV) redox couples.³⁶ Co_3O_4 has a special spinel structure in which one of the three Co atoms is in the Co(II) state, and the other two are in the Co(III) state. Under strong alkaline conditions, Co_3O_4 may be oxidized to CoOOH to catalytically oxidize glucose.

Li *et al.*³⁷ used CuCl_2 and CoCl_2 as raw materials to synthesize Co-MOF nanosheets on foamed nickel by a hydrothermal method. As can be seen in Fig. 6, the synthesized Co-MOF is an ultra-thin layered structure.³⁸ In an alkaline medium, the coordination interaction between Co^{2+} and organic molecules becomes weak, and the released Co^{2+} reacts with OH^- in solution to form CoOOH.³⁹ The reaction mechanism can be expressed by eqn (1)–(3):^{40–42}



Co-MOF/NiF is a glucose-sensitive material with excellent performance. The response range for glucose is 1–3000 μM , the sensitivity is 10 886 $\mu\text{A mM}^{-1} \text{cm}^{-2}$, and the detection limit is 1.3 nM. Table 3 summarizes the Co-based glucose sensors in the past three years and shows the key performance parameters in detail.

Table 2 List of Cu-based electrochemical non-enzymatic glucose sensors

Electrode materials	Sensitivity ($\mu\text{A mM}^{-1} \text{cm}^{-2}$)	Linear range (μM)	LOD (μM)	Operation potential (V)	Chemical environment	Ref.
CuS	13 620	160–11 760	2.72	0.50	0.1 M NaOH	28
Cu_2O	1470.85	1–700	—	0.50	0.1 M NaOH	30
Cu/CuO	33 950	1–5000	0.33	0.65	1.0 M NaOH	31
$\text{Cu}_2\text{O}/\text{CuO}$	1212.02, 852.80	10–200, 500–1600	—	0.40	0.5 M NaOH	32
Cu/CuS	5020	0.1–500	0.33	0.55	0.1 M NaOH	33

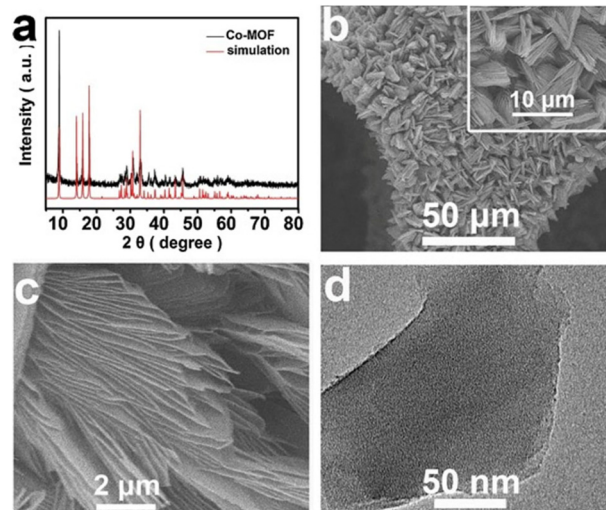


Fig. 6 (a) XRD pattern of Co-MOF and the synthesized Co-MOF sample. (b and c) SEM images. (d) HRTEM images.³⁷

4.2.3 Non-enzymatic glucose sensors based on nickel and its compounds. Similar to the above two metal elements, nickel and its compounds are also widely studied by scientists. Nickel based compounds are widely used in energy storage and electrocatalysis due to their low natural abundance, low cost and excellent electrochemical activity.⁴⁷ Their active centers mainly come from the redox pairs of Ni(II)/Ni(III) (Fig. 7).⁴⁸


Wang *et al.*⁴⁹ prepared composites (Ni/NiO/NG) in doped graphene by isolated air calcination. Ni/NiO/NG has a mixed valence state, and the special microporous scaffold structure provides a strong support force and responds well to glucose. The sensitivity of the Ni/NiO/NG electrode is 3251.8 $\mu\text{A mM}^{-1} \text{cm}^{-2}$ with a detection limit of 32 nM; in addition, the electrode also shows excellent selectivity, repeatability, long-term stability and high tolerance to chloride ions. Therefore, the Ni/NiO/NG non-enzymatic glucose sensor is expected to be a candidate for practical applications. Table 4 summarizes the Ni-based glucose sensors in the past three years and shows the key performance parameters in detail.

4.2.4 Non-enzymatic glucose sensor based on other transition metals and their compounds. As glucose sensitive material, the three transition metals mentioned above and their compounds are the most studied by researchers. In addition, some materials are also used in the field of glucose sensors, but there are few related reports, such as Zn,⁵⁵ Fe,⁵⁶ Mn,⁵⁷ *etc.* Their elemental or single oxides are not very



Table 3 List of Co-based electrochemical non-enzymatic glucose sensors

Electrode materials	Sensitivity ($\mu\text{A mM}^{-1} \text{cm}^{-2}$)	Linear range (μM)	LOD (μM)	Operation potential (V)	Chemical environment	Ref.
Co	10 886	1–3000	0.0013	0.50	0.1 M NaOH	37
Co ₃ O ₄	2550	1–122	0.28	0.50	0.1 M NaOH	43
CoTe ₂	16 800	10–5000	0.59	0.60	0.1 M NaOH	44
Co(OH) ₂	1646	0–3000	0.5	0.55	0.1 M KOH	45
Cu/Co(OH) ₂	42 700	1–250	0.073	0.50	0.1 M KOH	46

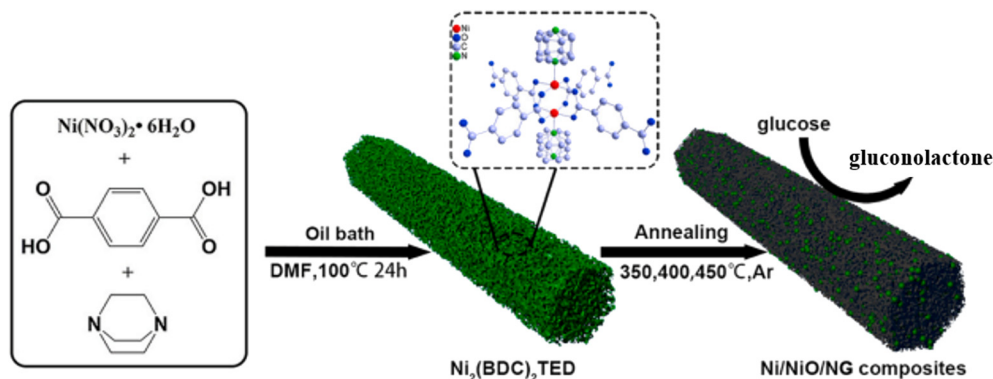**Fig. 7** The construction schematic of the Ni/NiO/NG nanocomposite electrode as well as the schematic of its glucose sensing mechanism.⁴⁹**Table 4** List of Ni-based electrochemical non-enzymatic glucose sensors

Electrode materials	Sensitivity ($\mu\text{A mM}^{-1} \text{cm}^{-2}$)	Linear range (μM)	LOD (μM)	Operation potential (V)	Chemical environment	Ref.
NiO	206.9	0.1–10 000	1.16	0.55	0.1 M KCl + 0.5 M NaOH	50
Ni(OH) ₂	11 171	1–400	—	0.60	0.1 M KOH	51
Ni–N–C	1181	1–1200	0.15	0.50	0.1 M NaOH	52
Ni(OH) ₂ /3DGF	2366	0.32–2200	0.32	0.40	0.2 M NaOH	53
Ni/Ni(OH) ₂	1078	200–6000	200	0.60	2.0 M NaOH	54

effective in the catalytic oxidation of glucose, but they can be combined with those with high catalytic properties to improve the performance by utilizing the synergistic relationship between different metal elements. In addition, transition metal based nitride,⁵⁸ phosphide,⁵⁹ sulfide²⁸ and selenide⁶⁰ are also commonly used catalyst materials for non-enzymatic glucose oxidation. Table 5 summarizes the non-enzymatic glucose sensors based on other transition metals and their compounds in recent years and shows the key performance parameters in detail.

4.3 Non-enzymatic glucose sensors with specific binding for glucose

In addition to the several sensitive materials described above, we can find a functional material that has a specific response

to glucose, such as boric acid and its derivatives, and a conductive polymer based on molecular imprinting technology (MIP), which has excellent selectivity for glucose molecules.

Kuivila *et al.*⁶⁶ first reported that phenylboronic acid and its derivatives could bind to sugars and form cyclic lactones in 1954, opening the door to the use of boric acid as a sugar recognition molecule. Lorand *et al.*⁶⁷ further studied the principle of binding between phenylboronic acid and sugar and pointed out that in an alkaline environment, the phenylboronic acid neutral molecule is converted to an anionic state, the boron atom is changed from sp^2 hybridization to sp^3 hybridization, and the boric acid configuration is changed from a planar triangle to a tetrahedral configuration. They also pointed out that boric acid could combine with 1,2- or 1,3-dihydroxy compounds to

Table 5 List of other transition metals-based electrochemical non-enzymatic glucose sensors

Electrode materials	Sensitivity ($\mu\text{A mM}^{-1} \text{cm}^{-2}$)	Linear range (μM)	LOD (μM)	Operation potential (V)	Chemical environment	Ref.
Cu–Ag–Zn	3572	0–6000	0.37	0.10	0.1 M NaOH	61
Ni–Al–Mn	2253	15–8000	1.49	0.80	0.1 M NaOH	62
Co–P/Cu	1818	500–2500	0.378	0.60	0.1 M KOH	63
SnO ₂	121.2	0.12–7800	0.04	0.90	0.1 M PBS (pH = 6)	64
Fe ₃ O ₄ /rGO	81.81	0–12 000	4.1	0.40	0.02 M PBS	65
	21.54	1000–19 000	2.2			



Table 6 List of boric acid and MIP-based electrochemical non-enzymatic glucose sensors

Electrode materials	Sensitivity	Linear range (μM)	LOD (μM)	Chemical environment	Ref.
MIP/CD	—	0.5–40, 50–600	0.09	0.05 M PBS	74
MIP	—	0.32–1000	0.19	0.1 M PBS (pH = 7.4)	75
GO-MIP	—	10–6000	0.02	PBS (pH = 5.0)	76

form a five- or six-membered cyclic lactone. The *cis-ortho*-dihydroxy group in the sugar ring structure has a stronger binding ability to boric acid than the simple chain-like *ortho*-dihydroxy compound (such as ethylene glycol). Therefore, boric acid can be used as a recognition site for saccharide sensors in the field of glucose detection. Liu *et al.*⁶⁸ presented a continuous glucose monitoring platform consisting of a quartz crystal microbalance (QCM) quartz and a flexible hydrogel recognition system. A stretchable hydrogel is employed as the support material and antifouling membrane, and glucose-sensitive monomer phenylboronic acid (PBA) is employed as the recognition part. The hydrogel membrane with PBA firmly adhered onto the electrode surface of the quartz crystal, and the lower limit of glucose detection of the platform was 0.15 mg L^{-1} .

MIT refers to the process of preparing a polymer with specific recognition for a specific target molecule,⁶⁹ it is a powerful technology for synthesizing high molecular type artificial receptors,⁷⁰ MIT has been widely used in the fields of chromatographic separation,⁷¹ chiral separation⁷² and sensing probe.⁷³ MIT-based polymers (MIP) have a selective response to target molecules of natural receptors,⁷⁴ and in MIP-based glucose sensors, a monomer having a functional moiety is polymerized with glucose to produce a specific polymer template for identifying glucose, which can be detected by reading an identification signal. MIP has high selectivity to glucose, good stability and low cost; however, MIP has a longer response time to glucose and is susceptible to external environments such as temperature and pH. There are currently few papers on the detection of glucose molecules. Table 6 summarizes the non-enzymatic glucose sensors based on boric acid and MIP in recent years and shows the key performance parameters in detail.

5 Summary

In this paper, we review the electrode materials available in non-enzymatic glucose sensors in recent years and their research status, including precious metals, transition metals, and substances that specifically respond to glucose. Precious metals have high electrocatalytic activity for glucose, but their sensitivity and stability are poor. Transition metal, represented by Cu, Co and Ni, have good electrocatalytic activity and stability for glucose, but the selectivity is poor, and the catalytic activity is greatly affected by nanomaterials. Electrode materials with a specific selectivity for glucose are too dependent on the balance between glucose and functional groups, the reaction conditions are harsh, and the linear range and stability need to be improved. We also need

to conduct deeper research to combine the advantages of materials to make up for their problems and shortcomings in sensing performance (Fig. 8).

6 Outlook

Since 2000, non-enzymatic glucose sensors have achieved tremendous development, and the number of articles on glucose sensors has been increasing year by year. In the past three years, the number of articles on glucose sensors on ScienceDirect is 1910 (2019), 2190 (2020), and 2804 (2021), indicating that there is still room and potential for the development of non-enzymatic glucose sensors. The development of nanomaterials and nanotechnology can provide more options and possibilities for the further development of glucose sensors.

Previously, the detection of glucose basically requires blood, which is a non-continuous invasive test. If we develop a non-invasive detection method to detect the concentration of glucose in the body, such as saliva,⁷⁷ tears,⁷⁸ sweat,⁷⁹ *etc.*, this will be a huge advancement in glucose detection technology and a huge boon for patients. At present, some research teams have tried in this direction. Garcia-Carmona *et al.*⁸⁰ designed a pacifier-type wireless device that can detect blood sugar levels by detecting the baby's saliva. Liu *et al.*⁸¹ reported a new device that can detect the amount of glucose in sweat. The team integrated highly sensitive In_2O_3 nanostrip field effect transistors (FETs) into substrates and devices for glucose detection. Non-intrusive sensors have too

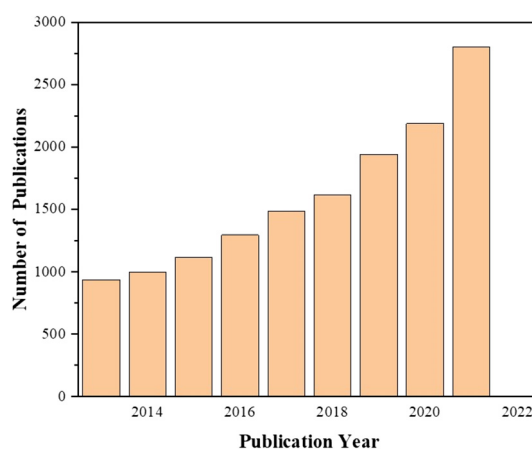


Fig. 8 Chart of the latest publications for enzyme-free glucose sensors as a function of year (results collected using the ScienceDirect database with the “non-enzymatic glucose sensors” as the search term).



many interference factors in the detection process, and the accuracy and repeatability are yet to be confirmed; besides, the correlation between saliva, tears, other fluids and blood glucose concentrations remains to be verified. Researchers need to conduct deeper research on the sensing mechanisms and influencing factors to provide more effective solutions for the development of commercial non-enzyme sensors.⁸²

This research did not receive any specific grant from funding agencies in the public, commercial, or not-for-profit sectors.

Conflicts of interest

There are no conflicts to declare.

References

- G. Lamprecht, F. Pichlmayer and E. R. Schmid, Determination of the authenticity of vanilla extracts by stable isotope ratio analysis and component analysis by HPLC, *J. Agric. Food Chem.*, 1994, **42**, 1722–1727.
- Y. Ni, G. Zhang and S. Kokot, Simultaneous spectrophotometric determination of maltol, ethyl maltol, vanillin and ethyl vanillin in foods by multivariate calibration and artificial neural networks, *Food Chem.*, 2005, **89**, 465–473.
- H. Kawakami, Y. Ito, Y.-A. Chien, C.-Y. Chen, W.-T. Chiu, P. Chakraborty, T. Nakamoto, M. Sone and T.-F. M. Chang, Development of polypyrrole/nano-gold composite for non-enzymatic glucose sensors, *Micro Nano Eng.*, 2022, **14**, 100109.
- E.-H. Yoo and S.-Y. Lee, *et al.*, Glucose Biosensors: An Overview of Use in Clinical Practice, *Sensors*, 2010, **10**, 4558–4576; E.-H. Yoo and S.-Y. Lee, *Sensors*, 2010, **10**, 1–2.
- A. Heller and B. Feldman, Electrochemistry in Diabetes Management, *Acc. Chem. Res.*, 2010, **43**, 963–973.
- C. Lyons, L. Clark, H. McDowell and K. McArthur, Cerebral Venous Oxygen Content During Carotid Thrombectomy, *Ann. Surg.*, 1964, **160**, 561–567.
- E. Ding, J. Hai, T. Li, J. Wu, F. Chen, Y. Wen, B. Wang and X. Lu, Efficient Hydrogen-Generation CuO/Co₃O₄ Heterojunction Nanofibers for Sensitive Detection of Cancer Cells by Portable Pressure Meter, *Anal. Chem.*, 2017, **89**, 8140–8147.
- D. Pletcher, *Electrocatalysis*, 1984, **14**, 403–415.
- L. D. Burke, Premonolayer oxidation and its role in electrocatalysis, *Electrochim. Acta*, 1994, **39**, 1841–1848.
- M. Sun, J. Liu, S. Wang, Z. Wang and X. Song, Solvothermal synthesis of hollow spherical CuCo₂O₄ as high-performance non-enzymatic glucose sensors, *Ionics*, 2021, **27**, 2257–2266.
- X. Liang, W. Li, H. Han and Z. Ma, Non-enzymatic electrochemical sensor based on Cu₂O/AuCu/Cu composite for hydrogen peroxide detection, *J. Electroanal. Chem.*, 2019, **834**, 43–48.
- B. Li, B. Luo, J. Zhao, Y. Pan, H. Zhou, Y. Xiao, S. Lei and B. Cheng, High electrical conductivity-induced enhancement effect of electrochemical performance in mesoporous NiCo₂S₄ nanorod-based supercapacitor, *J. Energy Storage*, 2019, **26**, 100955.
- Z. Cui, H. Yin, Q. Nie, D. Qin, W. Wu and X. He, Hierarchical flower-like NiO hollow microspheres for non-enzymatic glucose sensors, *J. Electroanal. Chem.*, 2015, **757**, 51–57.
- C. Wei, Q. Chen, C. Cheng, R. Liu, Q. Zhang and L. Zhang, Mesoporous nickel cobalt manganese sulfide yolk-shell hollow spheres for high-performance electrochemical energy storage, *Inorg. Chem. Front.*, 2019, **6**, 1851–1860.
- S. Park, T. D. Chung and H. C. Kim, Nonenzymatic Glucose Detection Using Mesoporous Platinum, *Anal. Chem.*, 2003, **75**, 3046–3049.
- S. Park, Y. J. Song, J.-H. Han, H. Boo and T. D. Chung, Structural and electrochemical features of 3D nanoporous platinum electrodes, *Electrochim. Acta*, 2010, **55**, 2029–2035.
- S. Biella, L. Prati and M. Rossi, Selective Oxidation of D-Glucose on Gold Catalyst, *J. Catal.*, 2002, **206**, 242–247.
- K. Shim, W.-C. Lee, M.-S. Park, M. Shahabuddin, Y. Yamauchi, M. S. A. Hossain, Y.-B. Shim and J. H. Kim, Au decorated core-shell structured Au@Pt for the glucose oxidation reaction, *Sens. Actuators, B*, 2019, **278**, 88–96.
- N. N. Shen, H. J. Xu, W. C. Zhao, Y. M. Zhao and X. Zhang, Highly Responsive and Ultrasensitive Non-Enzymatic Electrochemical Glucose Sensor Based on Au Foam, *Sensors*, 2019, **19**(5), 1203.
- A. Awais, M. Arsalan, X. Qiao, W. Yahui, Q. Sheng, T. Yue and Y. He, Facial synthesis of highly efficient non-enzymatic glucose sensor based on vertically aligned Au-ZnO NRs, *J. Electroanal. Chem.*, 2021, **895**, 115424.
- J. Cao, J. Yun, N. Zhang, Y. Wei, H. Yang and Z. Xu, Bifunctional Ag@Ni-MOF for high performance supercapacitor and glucose sensor, *Synth. Met.*, 2021, **282**, 116931.
- D.-W. Hwang, S. Lee, M. Seo and T. D. Chung, Recent advances in electrochemical non-enzymatic glucose sensors – A review, *Anal. Chim. Acta*, 2018, **1033**, 1–34.
- S. Berchmans, H. Gomathi and G. P. Rao, Electrooxidation of alcohols and sugars catalysed on a nickel oxide modified glassy carbon electrode, *J. Electroanal. Chem.*, 1995, **394**, 267–270.
- J. M. Marioli and T. Kuwana, Electrochemical characterization of carbohydrate oxidation at copper electrodes, *Electrochim. Acta*, 1992, **37**, 1187–1197.
- A. El Golli, M. Echabaane and C. Dridi, Development of an electrochemical nanoplatform for non-enzymatic glucose sensing based on Cu/ZnO nanocomposite, *Mater. Chem. Phys.*, 2022, **280**, 125844.
- W. Liu, X. Zhao, Y. Dai and Y. Qi, Preparation of three dimensional Cu₂O/Au/GO hybrid electrodes and its application as a non-enzymatic glucose sensor, *Microchem. J.*, 2022, **179**, 107451.
- L. Yang, J. Yang, Q. Dong, F. Zhou, Q. Wang, Z. Wang, K. Huang, H. Yu and X. Xiong, One-step synthesis of CuO nanoparticles based on flame synthesis: As a highly effective



- non-enzymatic sensor for glucose, hydrogen peroxide and formaldehyde, *J. Electroanal. Chem.*, 2021, **881**, 114965.
- 28 K. P. Sharma, M. Shin, G. P. Awasthi, M. B. Poudel, H. J. Kim and C. Yu, Chitosan polymer matrix-derived nanocomposite (CuS/NSC) for non-enzymatic electrochemical glucose sensor, *Int. J. Biol. Macromol.*, 2022, **206**, 708–717.
- 29 X. Liu, W. Yang, L. Chen and J. Jia, Three-Dimensional Copper Foam Supported CuO Nanowire Arrays: An Efficient Non-enzymatic Glucose Sensor, *Electrochim. Acta*, 2017, **235**, 519–526.
- 30 F. Sun and Z. Wang, Highly-branched dendrite cuprous oxide films for non-enzymatic amperometric glucose sensor, *Mater. Lett.*, 2019, **234**, 62–65.
- 31 L. Zhang, H. Liang, X. Ma, C. Ye and G. Zhao, A vertically aligned CuO nanosheet film prepared by electrochemical conversion on Cu-based metal-organic framework for non-enzymatic glucose sensors, *Microchem. J.*, 2019, **146**, 479–485.
- 32 S. Wang, L. Jiang, J. Hu, Q. Wang, S. Zhan and Y. Lu, Dual-functional Cu₂O/Cu electrodes for supercapacitors and non-enzymatic glucose sensors fabricated by femtosecond laser enhanced thermal oxidation, *J. Alloys Compd.*, 2020, **815**, 152105.
- 33 G.-R. Xu, C. Ge, D. Liu, L. Jin, Y.-C. Li, T.-H. Zhang, M. M. Rahman, X.-B. Li and W. Kim, In-situ electrochemical deposition of dendritic Cu-Cu₂S nanocomposites onto glassy carbon electrode for sensitive and non-enzymatic detection of glucose, *J. Electroanal. Chem.*, 2019, **847**, 113177.
- 34 V. R. Shinde, S. B. Mahadik, T. P. Gujar and C. D. Lokhande, Supercapacitive cobalt oxide (Co₃O₄) thin films by spray pyrolysis, *Appl. Surf. Sci.*, 2006, **252**, 7487–7492.
- 35 Q. Balouch, Z. H. Ibupoto, G. Q. Khaskheli, R. A. Soomro, S. S. Sirajuddin, M. K. Samoon and V. K. Deewani, Cobalt Oxide Nanoflowers for Electrochemical Determination of Glucose, *J. Electron. Mater.*, 2015, **44**, 3724–3732.
- 36 T. R. I. Cataldi, A. Guerrieri, I. G. Casella and E. Desimoni, Study of a cobalt-based surface modified glassy carbon electrode: Electrocatalytic oxidation of sugars and alditols, *Electroanalysis*, 1995, **7**, 305–311.
- 37 Y. Li, M. Xie, X. Zhang, Q. Liu, D. Lin, C. Xu, F. Xie and X. Sun, Co-MOF nanosheet array: A high-performance electrochemical sensor for non-enzymatic glucose detection, *Sens. Actuators, B*, 2019, **278**, 126–132.
- 38 J. Zhao, P. Su, Y. Zhao, M. Li, Y. Yang, Q. Yang and C. Li, Systematic morphology and phase control of Mg-ptcda coordination polymers by Ostwald ripening and self-templating, *J. Mater. Chem.*, 2012, **22**, 8470–8475.
- 39 P. Su, S. Liao, F. Rong, F. Wang, J. Chen, C. Li and Q. Yang, Enhanced lithium storage capacity of Co₃O₄ hexagonal nanorings derived from Co-based metal organic frameworks, *J. Mater. Chem. A*, 2014, **2**, 17408–17414.
- 40 C. Barbero, G. A. Planes and M. C. Miras, Redox coupled ion exchange in cobalt oxide films, *Electrochem. Commun.*, 2001, **3**, 113–116.
- 41 Q.-Q. Sun, M. Wang, S.-J. Bao, Y. C. Wang and S. Gu, Analysis of cobalt phosphide (CoP) nanorods designed for non-enzyme glucose detection, *Analyst*, 2016, **141**, 256–260.
- 42 Y. Ding, Y. Wang, L. Su, M. Bellagamba, H. Zhang and Y. Lei, Electrospun Co₃O₄ nanofibers for sensitive and selective glucose detection, *Biosens. Bioelectron.*, 2010, **26**, 542–548.
- 43 X. Lin, Y. Wang, M. Zou, T. Lan and Y. Ni, Electrochemical non-enzymatic glucose sensors based on nano-composite of Co₃O₄ and multiwalled carbon nanotube, *Chin. Chem. Lett.*, 2019, **30**, 1157–1160.
- 44 A. Farid, L. Pan, M. Usman, I. A. Khan, A. S. Khan, A. U. Ahmad and M. Javid, In-situ growth of porous CoTe₂ nanosheets array on 3D nickel foam for highly sensitive binder-free non-enzymatic glucose sensor, *J. Alloys Compd.*, 2021, **861**, 158642.
- 45 Y. Tao, Q. Liu, Q. Chang, J. Duan, Z. Tao, H. Guan, G. Chen, Y. Mao, J. Xie and C. Dong, In situ fabrication of Co(OH)₂ by hydrothermal treating Co foil in MOH (M = H, Li, Na, K) for non-enzymatic glucose detection, *J. Alloys Compd.*, 2019, **781**, 1033–1039.
- 46 L. Wang, S. Zhuang, L. Wang, N. Wang, H. Mo, Y. Tang, Y. Chen, Y. Sun and P. Wan, One step synthesis of hierarchical Cu nanoparticles-Co(OH)₂ nanoflakes/Nifoam electrode for ultrasensitive detection of glucose, *Appl. Surf. Sci.*, 2019, **467–468**, 773–781.
- 47 C. Wei, J. Sun, Y. Zhang, Y. Liu, Z. Guo, W. Du, L. Liu and Y. Zhang, Hierarchical Ni(OH)₂-MnO₂ hollow spheres as an electrode material for high-performance supercapacitors, *Inorg. Chem. Front.*, 2022, **9**, 3542–3551.
- 48 N. Salarizadeh, M. Habibi-Rezaei and S. J. Zargar, NiO-MoO₃ nanocomposite: A sensitive non-enzymatic sensor for glucose and urea monitoring, *Mater. Chem. Phys.*, 2022, **281**, 125870.
- 49 Q. Wang, S. Zheng, T. Li and Z. Wang, Ni/NiO multivalent system encapsulated in nitrogen-doped graphene realizing efficient activation for non-enzymatic glucose sensing, *Ceram. Int.*, 2021, **47**, 22869–22880.
- 50 C. Heyser, R. Schrebler and P. Grez, New route for the synthesis of nickel (II) oxide nanostructures and its application as non-enzymatic glucose sensor, *J. Electroanal. Chem.*, 2019, **832**, 189–195.
- 51 X. Zhong, Z. He, H. Chen and Y. Chen, Enhancing the non-enzymatic glucose detection performance of Ni(OH)₂ nanosheets via defect engineering, *Surf. Interfaces*, 2021, **25**, 101234.
- 52 X. Chen, X. He, J. Gao, J. Jiang, X. Jiang and C. Wu, Three-dimensional porous Ni, N-codoped C networks for highly sensitive and selective non-enzymatic glucose sensing, *Sens. Actuators, B*, 2019, **299**, 126945.
- 53 W. Mao, H. He, Z. Ye and J. Huang, Three-dimensional graphene foam integrated with Ni(OH)₂ nanosheets as a hierarchical structure for non-enzymatic glucose sensing, *J. Electroanal. Chem.*, 2019, **832**, 275–283.
- 54 E. M. Almutairi, M. A. Ghanem, A. Al-Warthan, M. R. Shaik, S. F. Adil and A. M. Almutairi, Chemical deposition and exfoliation from liquid crystal template: Nickel/nickel (II) hydroxide nanoflakes electrocatalyst for a non-enzymatic



- glucose oxidation reaction, *Arabian J. Chem.*, 2022, **15**, 103467.
- 55 F. Zhou, Y. Li, Y. Tang, F. Gao, W. Jing, Y. Du and F. Han, A novel flexible non-enzymatic electrochemical glucose sensor of excellent performance with ZnO nanorods modified on stainless steel wire sieve and stimulated via UV irradiation, *Ceram. Int.*, 2022, **48**, 14395–14405.
- 56 H. Shu, S. Peng, T. Lai, X. Cui, J. Ren, T. Chen, X. Xiao and Y. Wang, Nickel foam electrode decorated with Fe-CdIn₂O₄ nanoparticles as an effective electrochemical sensor for non-enzymatic glucose detection, *J. Electroanal. Chem.*, 2022, **919**, 116524.
- 57 Q. Dong, Z. He, X. Tang, Y. Zhang, L. Yang, K. Huang, X. Jiang and X. Xiong, One-step synthesis of Mn₃O₄@ZIF-67 on carbon cloth: As an effective non-enzymatic glucose sensor, *Microchem. J.*, 2022, **175**, 107203.
- 58 B. Zhang, L. Huang, X. Zhang, Y. Du, H. Sun, C. Jin, T. Zuo, L. He and W. Fa, Tantalum nitride nanotube structured electrode for non-enzymatic hydrogen peroxide sensing via photoelectrochemical route, *J. Electroanal. Chem.*, 2022, **912**, 116262.
- 59 L. He, J. Li, J. Cao, X. Li, X. Feng, J. Zhang and Y. Yang, High performance of non-enzymatic glucose biosensors based on the design of microstructure of Ni₂P/Cu₃P nanocomposites, *Appl. Surf. Sci.*, 2022, **593**, 153395.
- 60 Z. Rahmati, M. Roushani and H. Hosseini, Hierarchical hollow sea-urchin-like Ni-Co diselenide encapsulated in N-doped carbon networks as an advanced core-shell bifunctional electrocatalyst for fabrication of nonenzymatic glucose and hydrogen peroxide sensors, *Sens. Actuators, B*, 2020, **324**, 128730.
- 61 S. Liu, B. Liu, C. Gong and Z. Li, A nanoporous Cu-Ag thin film at the Cu-Ag-Zn alloy surface by spontaneous dissolution of Zn and Cu in different degrees as a highly sensitive non-enzymatic glucose sensor, *Electrochim. Acta*, 2019, **320**, 134599.
- 62 N. I. Chandrasekaran and M. Manickam, A sensitive and selective non-enzymatic glucose sensor with hollow Ni-Al-Mn layered triple hydroxide nanocomposites modified Ni foam, *Sens. Actuators, B*, 2019, **288**, 188–194.
- 63 H. Chen, P. Sun, M. Qiu, M. Jiang, J. Zhao, D. Han, L. Niu and G. Cui, Co-P decorated nanoporous copper framework for high performance flexible non-enzymatic glucose sensors, *J. Electroanal. Chem.*, 2019, **841**, 119–128.
- 64 C. Duan and J. Zheng, Porous coralloid Polyaniline/SnO₂-based enzyme-free sensor for sensitive and selective detection of nitrite, *Colloids Surf., A*, 2019, **567**, 271–277.
- 65 A. Ghosh, D. Ganguly and R. Sundara, A new approach to in-situ uniform growth of Fe₃O₄ nanoparticles over thermally exfoliated rGO sheet for the non-enzymatic and enzymatic detection of glucose, *J. Electroanal. Chem.*, 2021, **895**, 115386.
- 66 H. Kuivila, A. Keough and E. Soboczenski, Areneborates from diols and polyols, *J. Org. Chem.*, 1954, **19**, 780–783.
- 67 J. Lorand and J. Edwards, Polyol Complexes and Structure of the Benzeneboronate Ion, *J. Org. Chem.*, 1959, **24**(6), 769–774.
- 68 N. Liu, X. Xiang, M. Sun, P. Li, H. Qin, H. Liu, Y. Zhou, L. Wang, L. Wu and J. Zhu, Flexible hydrogel non-enzymatic QCM sensor for continuous glucose monitoring, *Biosens. Bioelectron.*, 2022, **10**, 100110.
- 69 S. Azad, M. Khosravi, A. Nikzad and S. K. Mishra, A novel contemporary molecular imprinting technique for non-enzymatic selective glucose detection, *Opt. Laser Technol.*, 2022, **148**, 107786.
- 70 T. Chen, A. Zhang, Y. Cheng, Y. Zhang, D. Fu, M. Liu, A. Li and J. Liu, A molecularly imprinted nanoreactor with spatially confined effect fabricated with nano-caged cascaded enzymatic system for specific detection of monosaccharides, *Biosens. Bioelectron.*, 2021, **188**, 113355.
- 71 T. Kubo and K. Otsuka, Recent progress in molecularly imprinted media by new preparation concepts and methodological approaches for selective separation of targeting compounds, *TrAC, Trends Anal. Chem.*, 2016, **81**, 102–109.
- 72 T. J. Ward and K. D. Ward, Chiral Separations: A Review of Current Topics and Trends, *Anal. Chem.*, 2012, **84**, 626–635.
- 73 L. Uzun and A. P. F. Turner, Molecularly-imprinted polymer sensors: realising their potential, *Biosens. Bioelectron.*, 2016, **76**, 131–144.
- 74 W. Zheng, H. Wu, Y. Jiang, J. Xu, X. Li, W. Zhang and F. Qiu, A molecularly-imprinted-electrochemical-sensor modified with nano-carbon-dots with high sensitivity and selectivity for rapid determination of glucose, *Anal. Biochem.*, 2018, **555**, 42–49.
- 75 D.-M. Kim, J.-M. Moon, W.-C. Lee, J.-H. Yoon, C. S. Choi and Y.-B. Shim, A potentiometric non-enzymatic glucose sensor using a molecularly imprinted layer bonded on a conducting polymer, *Biosens. Bioelectron.*, 2017, **91**, 276–283.
- 76 S. Alexander, P. Baraneedharan, S. Balasubrahmanyam and S. Ramaprabhu, Highly sensitive and selective non enzymatic electrochemical glucose sensors based on Graphene Oxide-Molecular Imprinted Polymer, *Mater. Sci. Eng., C*, 2017, **78**, 124–129.
- 77 D. Wang, C. Zheng, Y. Li, C. Han, H. Fang, X. Fang and H. Zhao, Sensitive non-invasive electrochemical sensing of glucose in saliva using amorphous SnO_x decorated one-dimensional CuO nanorods rich in oxygen vacancy defects, *Appl. Surf. Sci.*, 2022, **592**, 153349.
- 78 J. Zhu, S. Liu, Z. Hu, X. Zhang, N. Yi, K. Tang, M. G. Dexheimer, X. Lian, Q. Wang, J. Yang, J. Gray and H. Cheng, Laser-induced graphene non-enzymatic glucose sensors for on-body measurements, *Biosens. Bioelectron.*, 2021, **193**, 113606.
- 79 F. Vasiliou, A. K. Plessas, A. Economou, N. Thomaidis, G. S. Papaefstathiou and C. Kokkinos, Graphite paste sensor modified with a Cu(II)-complex for the enzyme-free simultaneous voltammetric determination of glucose and uric acid in sweat, *J. Electroanal. Chem.*, 2022, 116393.
- 80 L. Garcia-Carmona, A. Martin, J. R. Sempionatto, J. R. Moreto, M. C. Gonzalez, J. Wang and A. Escarpa, Pacifier



- Biosensor: Toward Noninvasive Saliva Biomarker Monitoring, *Anal. Chem.*, 2019, **91**(21), 13883–13891.
- 81 Q. Liu, Y. Liu, F. Wu, X. Cao, Z. Li, M. Alharbi, A. N. Abbas, M. R. Amer and C. Zhou, Highly Sensitive and Wearable In₂O₃ Nanoribbon Transistor Biosensors with Integrated
- On-Chip Gate for Glucose Monitoring in Body Fluids, *ACS Nano*, 2018, **12**, 1170–1178.
- 82 J. Zhang, Z. Kuang, H. Li, S. Li and F. Xia, Electrode surface roughness greatly enhances the sensitivity of electrochemical non-enzymatic glucose sensors, *J. Electroanal. Chem.*, 2022, **919**, 116541.

