



Cite this: *J. Anal. At. Spectrom.*, 2024, **39**, 1033

# Assessment of matrix effects induced by chloride, sulfate and dissolved organic carbon during Si isotope measurements by MC-ICP-MS under wet plasma conditions†

Sofía López-Urzúa,<sup>ID</sup>\*<sup>a</sup> Tu-Han Luu<sup>a</sup> and Louis Derry<sup>ab</sup>

Since 2006, with the development of an optimized methodology for silicon purification based on alkaline fusion followed by cation-exchange chromatography, silicon isotopes have been widely measured across diverse sample types. Nevertheless, this technique does not remove anions and dissolved organic carbon (DOC), leading to potential matrix effects. Notably, under dry plasma conditions, several studies have reported offset in the  $\delta^{30}\text{Si}$  value up to +1.4‰ when  $[\text{S}]/[\text{Si}] > 0.02$  (wt/wt) and +0.65‰ when  $[\text{DOC}]/[\text{Si}] > 1.75$ . Here, we examine the matrix effects induced by chloride, sulfate and dissolved organic carbon under wet plasma conditions. To achieve this, we doped the NBS-28 (NIST® RM 8546) solution, with varying amounts of sulfate and chloride and measured the  $\delta^{30}\text{Si}$  value in the doped solutions. To investigate the DOC matrix effect, we used the UV photolysis method to decompose the DOC within natural samples and then compared the resulting  $\delta^{30}\text{Si}$  values with those of untreated samples. Importantly, we did not observe any significant  $\delta^{30}\text{Si}$  offset outside the range of our long-term analytical precision ( $\pm 0.11\%$ , 2SD) attributed to chloride, sulfate, or DOC across a range of  $[\text{Cl}^-]/[\text{Si}] = 0.09$  to 5.65,  $[\text{SO}_4^{2-}]/[\text{Si}] = 0.09$  to 5.65 and  $[\text{DOC}]/[\text{Si}] = 0.08$  to 6.38. Even though no offset in  $\delta^{30}\text{Si}$  value is observed for DOC-contaminated samples, we recommend removal of DOC. We suggest that the matrix effect observed under dry plasma conditions can be primarily attributed to the use of introduction systems with desolvating membranes, followed by differences in the operating parameters and the absolute quantity of anions introduced into the plasma. Our study indicates that precise and accurate measurements ( $< 0.11\%$ , 2SD) can be reached for stable Si isotope ratios by MC-ICP-MS in wet plasma, with a larger tolerance to sample based-matrix effect induced by anion contamination compared to dry plasma.

Received 25th August 2023  
 Accepted 19th February 2024

DOI: 10.1039/d3ja00290j

rsc.li/jaas

## Introduction

Silicon isotopes were measured for the first time in the early 1950s by Reynolds and Verhoogen<sup>1</sup> using gas source spectrometry. With the advent and improvement of MC-ICP-MS, De la Rocha *et al.*<sup>2</sup> were able to accurately measure the  $^{29}\text{Si}/^{28}\text{Si}$  ratio in sponge spicules and diatoms but not the  $^{30}\text{Si}/^{28}\text{Si}$  ratio due to isobaric interferences ( $^{29}\text{SiH}^+$ ,  $^{14}\text{N}^{16}\text{O}^+$ ,  $^{14}\text{N}^{15}\text{NH}^+$ ,  $^{14}\text{N}^{14}\text{ND}^+$  on  $^{30}\text{Si}^+$ ). The development of higher performance MC-ICP-MS instruments such as the Nu Plasma 1700 and Thermo Finnigan Neptune, with higher mass resolving power made it possible to isolate spectral interferences and enable the measurement of both ratios.<sup>3</sup> Furthermore, the introduction of

new methodologies for Si purification by alkaline fusion and cationic chromatography<sup>4–6</sup> facilitated the determination of  $\delta^{30}\text{Si}$  with high precision ( $\approx \pm 0.14\%$ , 2 standard deviations (SD)).

Unfortunately, cationic ion exchange chromatography does not remove anions or dissolved organic carbon, which can lead to sample matrix-based effects. These effects are defined as unequal transmission efficiency of ions from the plasma ion source to the detectors resulting in inaccurate determination of the  $^{29}\text{Si}/^{28}\text{Si}$  and  $^{30}\text{Si}/^{28}\text{Si}$  ratios.<sup>7</sup> Matrix effects affecting silicon isotope measurements by MC-ICP-MS have been previously observed in several studies. Van Den Boorn *et al.*<sup>8</sup> reported a  $\delta^{30}\text{Si}$  offset of +1.4‰ when  $[\text{S}]/[\text{Si}] > 0.02$  (wt/wt) in samples from sulfur-rich rock. Chen *et al.*<sup>9</sup> tested the influence of sulfur by doping a pure silicon solution and reported a similar  $\delta^{30}\text{Si}$  shift of +1.04‰ when  $[\text{S}]/[\text{Si}] > 0.02$ . Hughes *et al.*<sup>10</sup> observed a shift of +0.28‰ in river samples when  $[\text{SO}_4^{2-}]/[\text{Si}] > 0.35$ , as well as an offset of +0.29‰ and +0.65‰ produced by dissolved organic carbon when  $[\text{DOC}]/[\text{Si}] > 0.69$  and 1.75 respectively.

<sup>a</sup>Institut de Physique Du Globe de Paris, Université Paris Cité, CNRS, F-75005, Paris, France. E-mail: lopezurzua@ipgp.fr

<sup>b</sup>Department of Earth and Atmospheric Sciences, Cornell University, Ithaca, NY, USA

† Electronic supplementary information (ESI) available. See DOI: <https://doi.org/10.1039/d3ja00290j>



Table 1 Operating parameters for this work and studies that have tested the influence of DOC and anions ( $\text{Cl}^-$ ,  $\text{SO}_4^{2-}$ )

Parameters	This study	Georg <i>et al.</i> <sup>5</sup> (2006)	Van Den Boorn <i>et al.</i> <sup>8</sup> (2009) <sup>a</sup>	Hughes <i>et al.</i> , <sup>10</sup> (2011)	Chen <i>et al.</i> , <sup>9</sup> (2016)	Oelze <i>et al.</i> , <sup>11</sup> (2016)
Instrument	Thermo Finnigan Neptune Plus	Nu plasma 1700	Thermo Finnigan Neptune	Nu plasma	Nu plasma II	Thermo Finnigan Neptune
RF power (W)	1200	1300	n.i. <sup>b</sup>	n.i.	n.i.	n.i.
Resolution mode	Medium	High	Medium or high	Medium	Medium	High
Mass resolution	>4000	2000	2500	n.i.	4000	n.i.
Plasma type	Wet	Dry	Dry	Dry	Dry	Dry
Cool gas ( $\text{L min}^{-1}$ )	15–16	13	n.i.	n.i.	n.i.	n.i.
Auxiliary gas ( $\text{L min}^{-1}$ )	0.9–1.01	0.9–0.75	n.i.	n.i.	n.i.	n.i.
Sample gas ( $\text{L min}^{-1}$ )	0.98–1.1	n.i.	n.i.	n.i.	n.i.	n.i.
Introduction system	Cyclonic spray chamber	DSN-100 Nu instrument	Cetac Aridius	Cetac Aridius II + spray chamber	Cetac Aridius II	ESI Apex-Q without desolvation membrane
Nebulizer	PFA nebulizer (ESI)	N <sub>2</sub> ; n.i.	N <sub>2</sub> ; n.i.	N <sub>2</sub> ; n.i.	N <sub>2</sub> ; n.i.	N <sub>2</sub> ; no
Nebulizer uptake flow ( $\mu\text{L min}^{-1}$ )	≈100	Self-aspirant 6 mm microflow PFA nebulizer	PFA micro-concentric nebulizer	PFA nebulizer	PFA nebulizer	PFA nebulizer
Cones (sample and skimmer)	Jet and H	60–80	n.i.	n.i.	n.i.	100
Cup configuration	L4 ( <sup>28</sup> Si), L1 ( <sup>29</sup> Si), H2( <sup>30</sup> Si)	“Experimental” WA cone “Experimental” WA cone L7 ( <sup>29</sup> Al), L4 ( <sup>28</sup> Si), H1 ( <sup>29</sup> Si), H6 ( <sup>30</sup> Si)	L4 ( <sup>28</sup> Si), L1 ( <sup>29</sup> Si), C ( <sup>30</sup> Si)	n.i.	n.i.	L4 ( <sup>28</sup> Si), L1 ( <sup>29</sup> Si), C ( <sup>30</sup> Si), L2 ( <sup>24</sup> Mg), C ( <sup>25</sup> Mg) H3 ( <sup>26</sup> Mg)
Si concentration (ppm)	1	0.6	2–5	2	n.i.	0.8–1
Sensitivity on <sup>28</sup> Si (V per ppm)	9–11	13	6	n.i.	n.i.	6
Data acquisition	25 cycles, integration time of 4.194 s	25 cycles, integration time of 8 s	60 cycles, integration time of 4 s	n.i.	80 cycles, integration time of 5 s	Dynamic measurement (Mg-doping). 30 cycles, integration time of 4 s
Mg doping	No	No	No	Yes	No	Yes
Anion mass bias offset in $\delta^{30}\text{Si}$	Not observed	Not observed: up to $[\text{SO}_4^{2-}]/[\text{Si}] = 14.4$	+1.4% <sub>00</sub> , when $[\text{SO}_4^{2-}]/[\text{Si}] > 0.2$	+0.28% <sub>00</sub> , when $[\text{SO}_4^{2-}]/[\text{Si}] > 0.35$ +0.65% <sub>00</sub> , when $[\text{DOC}]/[\text{Si}] > 1.75$	+1.04% <sub>00</sub> , when $[\text{Si}]/[\text{Si}] > 0.25$	Not observed
Matrix	0.2 N HNO <sub>3</sub>	0.1 N HCl	0.25 N HNO <sub>3</sub>	HCl	HCl	0.1 N HCl

<sup>a</sup> Also based on Van Den Boorn *et al.* (2006). <sup>b</sup> n.i.: no information.

Conversely, Georg *et al.*<sup>5</sup> tested the effect of sulfates and nitrates on the accuracy of Si isotope measurements, but no significant isotopic effect was reported. Moreover, Oelze *et al.*<sup>11</sup> using Mg as an internal standard, doped the pure Si standard solution NBS-28 with different amounts of  $\text{NO}_3^-$ ,  $\text{SO}_4^{2-}$  and  $\text{PO}_4^{3-}$  and found no significant deviation from the expected value of 0%. Recently, Gaspard *et al.*<sup>12</sup> suggested the addition of an anionic column separation step for hydrothermal waters ( $[\text{SO}_4^{2-}]/[\text{Si}] > 2$ ) to remove the  $\text{SO}_4^{2-}$  impurities, but this requires samples with at least  $8 \text{ mg L}^{-1}$  of Si which are not always available in stream water. To the best of our knowledge, all the tests demonstrating sample matrix-based effects associated either with anions or DOC have been performed using 'dry' plasma conditions (refer to Table 1). The term 'dry', as defined by O'Connor *et al.*,<sup>13</sup> refers to the use of desolvation units to reduce the solvent load before the analyte enters the plasma. Although 'dry' plasma offers the benefit of increasing sensitivity, it also exacerbates matrix effects due to the preconcentration of both the matrix and the analyte.<sup>14</sup> In contrast, in 'wet' plasma, both the liquid phase aerosol and the vapor phase water are present. Isotopic measurements using 'wet' plasma require higher concentrations of Si, which may not always be possible depending on the type of samples but has the advantage of being less impacted by matrix effects. Consequently, the aim of this technical note is to investigate whether the sample matrix-based interferences observed in previous studies are also observed when Si isotopes are measured using a 'wet' plasma.

## Methods

### Materials and sample preparation

To investigate the potential impact of anions on the accuracy and precision of Si isotope measurements by MC-ICP-MS, we

doped the NBS-28 (NIST® RM 8546) solution, a pure silicon dioxide used as an international reference material, with varying amounts of (a)  $\text{Cl}^-$ , (b)  $\text{SO}_4^{2-}$  and (c) a mix of both anions at 1 : 1 ratio. We did not investigate the effect of nitrate in this study since the measurements were conducted in a 0.2 N  $\text{HNO}_3$  medium. The doping was achieved using dilutions of AccuSPEC SCP Science® ( $1001 \mu\text{g mL}^{-1}$ ) chloride and sulfate ion chromatography standards. We prepared a total of 36 doped samples, with  $[\text{anion}]/[\text{Si}]$  ratios ranging from 0.09 to 5.65, and then processed them through cationic chromatography – see details below.

To assess the potential effect of dissolved organic carbon on Si isotope measurements, we opted for natural solutions (stream, groundwater, and soil solutions) with varying amounts of DOC, rather than adding a DOC standard to the NBS-28 pure Si solution. The natural water samples were collected from three different catchments: the Weierbach experimental catchment in Luxembourg,<sup>15</sup> the Strengbach catchment<sup>16</sup> and the Kervidy-Naizin of the ArgHyS observatory,<sup>17</sup> both located in France. A total of 14 samples were selected to cover a large range of  $[\text{DOC}]/[\text{Si}]$  ratios, from 0.08 to 6.38, as shown in Table 2.

Soil solution, stream and groundwater samples were filtered through  $0.22 \mu\text{m}$  PES filters and collected in pre-cleaned LDPE bottles. Subsequently, the samples were acidified using concentrated 16 N  $\text{HNO}_3$  to reach pH 2. An additional 30 mL aliquot was filtered through a  $0.45 \mu\text{m}$  glass fiber filter and acidified with 3 drops of  $\text{H}_3\text{PO}_4$  in a glass bottle to determine the dissolved organic carbon. The samples were then stored refrigerated at  $3 \text{ }^\circ\text{C}$  until being processed in the clean labs at the Institut de physique du globe de Paris (IPGP, France). Silicon concentrations were measured using an Agilent 7900 Inductively Coupled Plasma source Mass Spectrometer (ICP-MS); spectral interferences on mass 28 were mitigated by the use of

**Table 2** Concentration of anions, silicon, DOC, and  $[\text{anion}]/[\text{Si}]$  ratios of the water samples from the different catchments investigated in this study

Water type	Sample name	Concentrations (ppm)				Ratios (ppm/ppm)		
		Si	DOC	$\text{Cl}^-$	$\text{SO}_4^{2-}$	$[\text{DOC}]/[\text{Si}]$	$[\text{Cl}^-]/[\text{Si}]$	$[\text{SO}_4^{2-}]/[\text{Si}]$
<b>Weierbach (Luxembourg)</b>								
Groundwater	GW11	6.68	0.531	3.917	10.724	0.08	0.59	1.60
Groundwater	GW5	2.74	0.927	3.920	6.454	0.34	1.43	2.36
Groundwater	GW2	2.86	2.355	3.090	6.993	0.82	1.08	2.44
Streamwater	SW2	2.64	2.863	3.399	6.092	1.09	1.29	2.31
Groundwater	GW9	2.87	4.000	3.340	9.374	1.39	1.16	3.26
Streamwater	SW3	2.54	3.721	3.190	7.080	1.47	1.26	2.79
<b>Strengbach (France)</b>								
Groundwater	CS2	4.17	0.773	2.363	3.558	0.19	0.57	0.85
Soil solution	RAZS	3.72	1.823	2.206	3.953	0.49	0.59	1.06
Groundwater	SG	2.78	2.060	2.070	4.361	0.74	0.75	1.57
Groundwater	BH	3.71	4.887	2.364	3.829	1.32	0.64	1.03
Streamwater	RUZS	1.78	9.186	1.291	1.159	5.16	0.73	0.65
<b>Kervidy-Naizin (France)</b>								
Streamwater	N1_Ech04	3.51	7.089	30.37	7.63	2.02	8.65	2.17
Streamwater	N1_Ech07	3.23	9.777	25.63	8.32	3.03	7.94	2.58
Streamwater	N1_Ech19	3.35	13.680	26.93	9.69	4.09	8.05	2.89



an integrated collision cell with He. DOC concentrations were determined using a Shimadzu TOC-VCSH Total Organic Carbon Analyzer. Both analytical instruments are located at IPGP.

To decompose the DOC present in the samples, we opted for a different method than the photo-ozonolysis used by Hughes *et al.*<sup>10</sup> Instead, we chose a UV photolysis method. To this end, 10 mL of acidified water samples were first transferred into a quartz vial (Metrohm) and 20  $\mu\text{L}$  of 30%  $\text{H}_2\text{O}_2$  (Suprapur) were added. The samples were irradiated using a UV digester (Metrohm AG – 705 UV Digester, equipped with a mercury lamp) at wavelength ranging from 200 to 600 nm for 10 minutes, followed by a cooling period of 10 minutes. This process was repeated twice, without adding any extra  $\text{H}_2\text{O}_2$ . After this treatment, the DOC concentration was measured to check the DOC decomposition. All samples had a post-treatment concentration below 0.5 ppm. We also conducted procedural blanks of ultrapure MilliQ water with 20  $\mu\text{L}$  of 30%  $\text{H}_2\text{O}_2$  to assess the degree of Si leaching from the quartz tubes and the purity of the  $\text{H}_2\text{O}_2$ . There was no evidence of Si contamination, as the Si concentration in the blanks was below the detection limit.

### Sample digestion

We used an alkali fusion technique adapted from the method published in Georg *et al.*<sup>5</sup> to digest five reference materials: NBS-28 (NIST® RM 8546), a pure silicon dioxide used as the bracketing standard; two USGS basalts, BHVO-2 (Hawaiian Volcano Observatory Basalt) and BCR-2 (Columbia River Basalt); an artificial highly fractionated  $\text{SiO}_2$  material known as Big Batch, which was prepared by precipitating large amounts of dissolved sodium metasilicate at the Marine Science Institute, UCSB, USA,<sup>18</sup> and a natural diatomite rock called “Diatomite”, which was obtained from one of the world’s largest diatomite deposits situated in Lompoc, California.<sup>19</sup> Ultrapure MilliQ® water (18.2 M $\Omega$  cm, Millipore, USA) was used for all the dilutions, and concentrated acids were purified by in-house sub-boiling distillation. For each reference material, depending on the Si concentration, we weighed between 5 mg and 10 mg of powdered material in Ag crucibles and added NaOH pellets (analytical grade, Merck) while maintaining a ratio between the material’s weight and the NaOH pellets of less than 1 : 10. The crucibles were heated at 720 °C for 12 minutes in a muffle furnace, and left to cool down to 300 °C. Subsequently, the crucibles were transferred into a Teflon vial with 15 mL of MilliQ® water, closed and left for 24 hours at room temperature. The liquid was then transferred into LDPE bottles, and the Teflon vial containing the crucibles was filled with 10 mL of MilliQ® water and sonicated for 15 minutes before transferring the liquid into the bottle. This step was repeated three times to ensure optimal recovery from the crucibles. Finally, the sample was diluted to reach a Si concentration of less than 30 ppm (to avoid precipitation of silica) and adjusted to 0.2 N  $\text{HNO}_3$ , ready for Si purification. The yields after alkaline fusions for standard are 94.5% for the NBS-28, 99.3% for BCR-2 and, 92.2% for BHVO-2. Uncertainties in powder weights (10–5 mg), dilution steps, and ICP-MS measurement are estimated at 3%.

### Chemical purification

The Si purification procedure involved a column chemistry protocol adapted from Van Den Boorn *et al.*<sup>6</sup> and Georg *et al.*<sup>5</sup> About 20  $\mu\text{g}$  Si were loaded onto a Biorad polypropylene column filled with 1.8 mL of AG50W-X12 resin (200–400 mesh). Silicon was eluted by adding 5 mL of MilliQ® water, in two steps. Approximately 70% of the silicon is collected in the first elution step (2 mL MilliQ®) with the remaining 30% being collected in the final elution step (3 mL MilliQ®). The solution is then adjusted to 0.2 N  $\text{HNO}_3$  and diluted for a target concentration of 1 ppm, ready to be analyzed on the MC-ICP-MS.

### Silicon isotope measurements by MC-ICP-MS

Silicon isotopes were measured using a Thermo Finnigan Neptune Plus MC-ICP-MS (IPGP, France) in ‘wet’ plasma mode. Samples were introduced using a Stable Introduction System (SIS) composed of a quartz spray chamber, with an uptake rate of  $\sim 100 \mu\text{L min}^{-1}$ . Jet sampler and H skimmer nickel cones were used. Isotopes  $^{28}\text{Si}$ ,  $^{29}\text{Si}$  and  $^{30}\text{Si}$  were simultaneously collected in three Faraday cups (L4, L1 and H2, respectively), using ‘medium’ resolution ( $M/\Delta M$  5–95% peak height  $\geq \sim 4000$ ) to separate polyatomic interferences. Table 1 shows the operating parameters of the Neptune Plus instrument used in the course of this study. The samples were analyzed at a silicon concentration of 1 ppm, with typical signal intensities for  $^{28}\text{Si}^+$  ranging from 9 to 11 V. The typical background signal on  $^{28}\text{Si}^+$  was  $< 0.04$  V. The Faraday cup amplifiers (with  $10^{11} \Omega$  feedback resistors) were internally calibrated for baseline and gain at the beginning of each analytical session. Silicon isotopic compositions are reported in standard per mil notation,  $\delta^{30}\text{Si}$  (‰) and  $\delta^{29}\text{Si}$  (‰), calculated by a classical standard-sample bracketing (SSB) method using the NBS-28 as the bracketing standard. One measurement consists of 25 cycles of 4.194 s integration. Each sample was measured multiple times ( $n$ ), and the reported delta values correspond to the average of the  $n$  consecutive measurements ( $n = 4$  to 8).

## Results and discussion

### Data quality and rejection criteria

The measurements were conducted over the course of three years (2021, 2022 and 2023). Certified USGS basalt standards

**Table 3**  $\delta^{30}\text{Si}$  and  $\delta^{29}\text{Si}$  values from replicate measurements of BHVO-2, Diatomite and Big Batch standards and the associated 2SD (two standard deviation) and their 95% confidence intervals ( $\text{CI} = t \times \text{SD}/\sqrt{n}$ ), with  $t$  critical value of a Student’s  $t$ -distribution over a 95% confidence

Standard name	$\delta^{30}\text{Si}$ (‰)			$\delta^{29}\text{Si}$ (‰)			$n$
	Mean	2SD	95% CI	Mean	2SD	95% CI	
BHVO-2	−0.30	0.12	0.01	−0.16	0.08	0.01	127
BCR-2	−0.28	0.12	0.05	−0.15	0.07	0.03	8
Diatomite	1.29	0.17	0.01	0.66	0.13	0.01	127
Big Batch	−10.59	0.20	0.03	−5.43	0.13	0.02	49



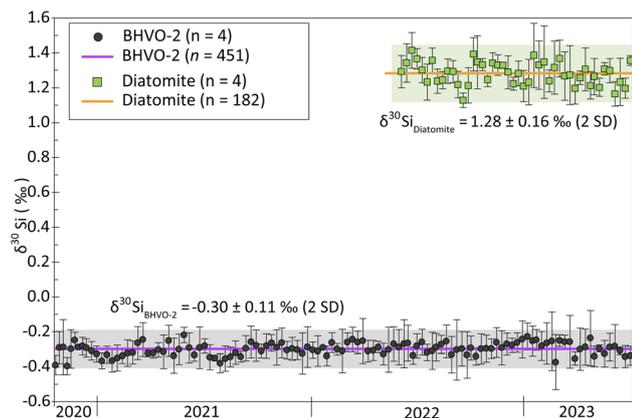


Fig. 1 Long-term reproducibility and short-term repeatability of BHVO-2 and Diatomite over three years. Green squares (Diatomite) and black dots (BHVO-2) represents the average values for 4 consecutive measurements, with error bars indicating the 95% CI. The long-term  $\delta^{30}\text{Si}$  in purple for BHVO-2 and orange for Diatomite represent the mean of all the measurements. Shaded areas around the lines represent the uncertainty (2SD).

BHVO-2 and BCR-2, Diatomite and Big Batch were routinely measured during the different analytical sessions to check the accuracy and precision of the measurements. Table 3 provides the  $\delta^{30}\text{Si}$  values obtained over the course of this study for these four reference materials, with  $\delta^{30}\text{Si} = -0.30 \pm 0.12\text{‰}$  (2SD,  $n = 127$ ) for BHVO-2,  $-0.28 \pm 0.12\text{‰}$  (2SD,  $n = 8$ ) for BCR-2,  $1.29 \pm 0.17\text{‰}$  (2SD,  $n = 127$ ) for Diatomite and  $-10.59 \pm 0.20\text{‰}$  (2SD,  $n = 49$ ) for Big Batch. The  $\delta^{30}\text{Si}$  obtained for BHVO-2 is in agreement with the value of  $-0.27 \pm 0.11\text{‰}$  (2SD) reported by Jochum *et al.*<sup>20</sup> based on a compilation of the GeoReM database, as well as with the more recent compilation of published data by Delvigne *et al.*,<sup>21</sup> which gave a value of  $-0.28 \pm 0.08\text{‰}$  (2SD). The  $\delta^{30}\text{Si}$  value for BCR-2 agree with compilation of 4 measurements in the GeoReM database with value of  $-0.24 \pm 0.05\text{‰}$  (2SD)

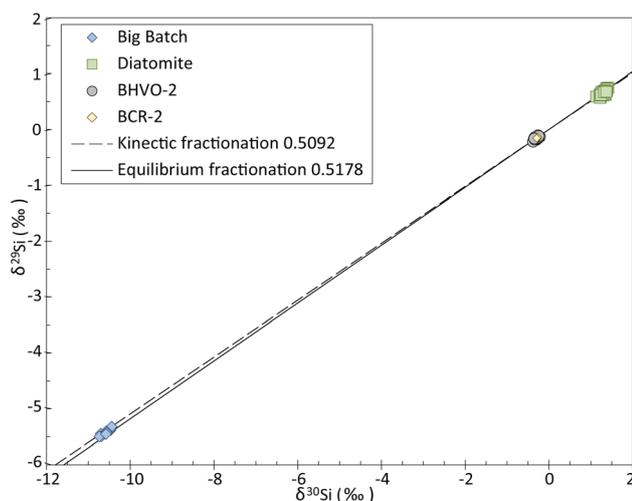


Fig. 2 Three-isotope plot of Si for the four reference materials BHVO-2, BCR-2, Big Batch and Diatomite measured during this study. Our data fall along a mass-dependent fractionation line with a slope of 0.5126 ( $\delta^{29}\text{Si} = \delta^{30}\text{Si} \times 0.5126$ ).

reported by Jochum *et al.*<sup>20</sup> The  $\delta^{30}\text{Si}$  values obtained for Diatomite and Big Batch are in good agreement with the values reported in Reynolds *et al.*,<sup>19</sup> who gave  $\delta^{30}\text{Si}$  values of  $1.26 \pm 0.20\text{‰}$  and  $-10.48 \pm 0.20\text{‰}$  respectively.

Additionally, the  $\delta^{30}\text{Si}$  values reported for BHVO-2 and Diatomite in this study are consistent with the long-term values we obtained over three years, comprising 14 analytical sessions for BHVO-2 and one year with 4 analytical sessions for Diatomite. Fig. 1 illustrates both the short-term repeatability (3 to 4 consecutive measurements) and the long-term reproducibility. Short-term repeatability for BHVO-2 and Diatomite is typically *ca.*  $0.07\text{‰}$  and  $0.09\text{‰}$  (95% CI), respectively. The long-term  $\delta^{30}\text{Si}$  values are  $-0.30 \pm 0.11\text{‰}$  (2SD,  $n = 451$ ) for BHVO-2 and  $-1.28 \pm$

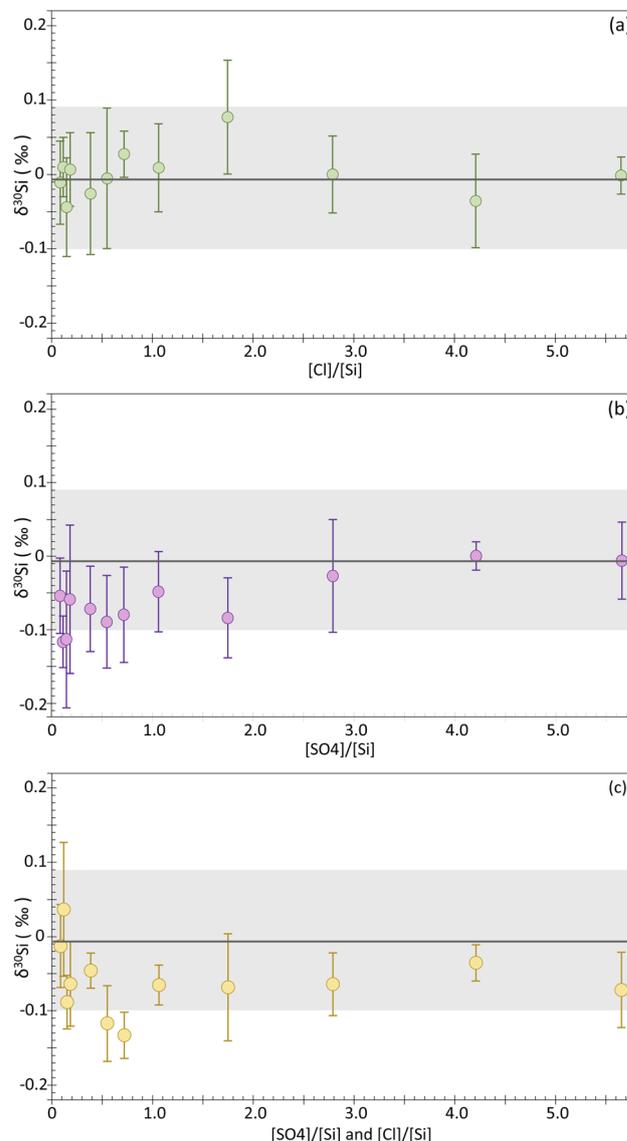


Fig. 3  $\delta^{30}\text{Si}$  values for the NBS-28 standard solution doped with chloride (a), sulfate (b) and both sulfate and chloride (c) at different [anion]/[Si] ratios. In each plot, error bars represent the 95% confidence interval for each sample, grey line represent the value of NBS-28 without doping ( $n = 97$ ) and the shaded area represent the uncertainty of  $0.09\text{‰}$  (2SD).



0.16‰ (2SD,  $n = 182$ ) for Diatomite, showing long-term reproducibility of 0.11‰ and 0.16‰ (2SD), respectively.

Analytical sequences in which the delta values of the reference standard were not in the margins of the long-term standard measurements were rejected. Likewise, samples whose 2SD were larger than 0.16 (average long-term 2SD for standards) were discarded and re-measured.

The three-isotope plot of Si (Fig. 2) shows that all the data obtained in this study plot along the mass-dependent fractionation line. The slope of the line described by our measurements is of  $0.5126 \pm 0.0032$  SE, calculated using IsoplotR's maximum likelihood estimator,<sup>22</sup> which is consistent with the slopes of the theoretical mass-dependent fractionation lines, *i.e.*, 0.5092 and 0.5178 for kinetic and equilibrium fractionation, respectively.

### Sulfate and chloride matrix effect

A total of 36 solutions of NBS-28 doped with anions were analyzed (12 with chloride, 12 with sulfate, and 12 with a mixture both at a 1:1 concentration ratio). Additionally, undoped NBS-28 was systematically measured during the different analytical sessions. Undoped NBS-28 was measured a total of 97 times, giving  $\delta^{30}\text{Si} = -0.01 \pm 0.09\text{‰}$  and  $\delta^{29}\text{Si} = 0.00 \pm 0.09\text{‰}$  (2SD), as expected for a self-bracketed solution. Overall, the 36 doped solutions show good reproducibility, with a 95% CI < 0.10‰ and 2SD < 0.14‰ for  $\delta^{30}\text{Si}$ . The results for each solution are reported in the ESI (Table A†), as well as in Fig. 3 where the  $\delta^{30}\text{Si}$  for each doped sample is plotted against the [anion]/[Si] ratio (wt/wt). Deviation from the  $\delta^{30}\text{Si}$  NBS-28 value of 0.0‰ would be observed if a matrix effect occurs. However, as can be seen on Fig. 2a, our chloride-doped solutions show no significant offset, with all the  $\delta^{30}\text{Si}$  values falling within the 2SD range of the undoped NBS-28. The  $\delta^{30}\text{Si}$  values for all doped solutions typically range from  $-0.04$  to  $0.03\text{‰}$ , with the exception of the solution whose  $[\text{Cl}^-]/[\text{Si}] = 1.75$  which has a  $\delta^{30}\text{Si}$  of  $0.08 \pm 0.08\text{‰}$  (95% CI). However, the latter value remains within uncertainties of the undoped NBS-28. Our results clearly indicate that no significant matrix effect is induced by the presence of chloride for  $[\text{Cl}^-]/[\text{Si}]$  ratio < 5.65. In contrast to the findings of Van Den Boorn *et al.*,<sup>8</sup> Chen *et al.*<sup>9</sup> and Hughes *et al.*,<sup>10</sup> we did not observe significant offset in the delta values resulting from  $\text{SO}_4^{2-}$  contamination or both  $\text{Cl}^-$  and  $\text{SO}_4^{2-}$  contamination. In general, the  $\delta^{30}\text{Si}$  values for the sulfate-doped solutions typically range from 0 to  $-0.09\text{‰}$ , with the exceptions of the solutions whose  $[\text{SO}_4^{2-}]/[\text{Si}] = 0.12$  and 0.15 that show a slightly larger deviation of  $-0.12\text{‰}$  and  $-0.11\text{‰}$ , respectively. However, all those values remain within uncertainties of the undoped NBS-28. Similarly, the solutions doped with both  $\text{Cl}^-$  and  $\text{SO}_4^{2-}$  anions show a similar behavior, with  $\delta^{30}\text{Si}$  values typically ranging from 0.04 to  $-0.09\text{‰}$ , except for the solutions whose  $[\text{SO}_4^{2-}]/[\text{Si}]$  and  $[\text{Cl}^-]/[\text{Si}] = 0.55$  and 0.72, which display a slightly larger deviation of  $-0.12\text{‰}$  and  $-0.13\text{‰}$  of  $\delta^{30}\text{Si}$ , respectively. Again, all those values remain within uncertainties of the undoped NBS-28.

To further evaluate the effect of anions on the precision and accuracy of Si isotope measurements, we divided all

Table 4 Mean of  $\delta^{30}\text{Si}$  and  $\delta^{29}\text{Si}$  values for the 4 groups and the associated 2SD and their 95% confidence intervals (CI =  $t \times \text{SD}/\sqrt{n}$ ). Results of the *T*-test for the combination for all groups, *t* represents the *t*-statistic and *p* value the probabilistic significance

Group	$\delta^{30}\text{Si}$ (‰)			$\delta^{29}\text{Si}$ (‰)			<i>n</i>
	Mean	2SD	95% CI	Mean	2SD	95% CI	
Undoped NBS-28	-0.01	0.09	0.01	0.00	0.09	0.01	97
$\text{Cl}^-$ doped	-0.00	0.09	0.01	0.01	0.07	0.01	48
$\text{SO}_4^{2-}$ doped	-0.06	0.10	0.01	-0.02	0.09	0.01	48
$\text{SO}_4^{2-}$ and $\text{Cl}^-$ doped	-0.06	0.12	0.01	-0.03	0.11	0.01	74
<i>T</i> test							
Group 1	Group 2	<i>t</i>	<i>P</i> values	Meaning			
Undoped NBS-28	$\text{Cl}^-$ doped	-0.55	0.58	Null hypothesis is accepted			
Undoped NBS-28	$\text{SO}_4^{2-}$ doped	5.12	0.00	Null hypothesis is rejected			
Undoped NBS-28	$\text{SO}_4^{2-}$ and $\text{Cl}^-$ doped	5.06	0.00	Null hypothesis is rejected			
$\text{Cl}^-$ doped	$\text{SO}_4^{2-}$ doped	6.25	0.00	Null hypothesis is rejected			
$\text{Cl}^-$ doped	$\text{SO}_4^{2-}$ and $\text{Cl}^-$ doped	6.18	0.00	Null hypothesis is rejected			
$\text{SO}_4^{2-}$ and $\text{Cl}^-$ doped	$\text{SO}_4^{2-}$ doped	-0.01	0.99	Null hypothesis is accepted			

measurements in four groups, as the  $\delta^{30}\text{Si}$  for the doped samples was consistent regardless of the [anion]/[Si] ratios. The first group consists of all the measurements of the undoped NBS-28 solution, while the second, third and fourth groups include measurements of samples doped with either chloride, or sulfate, or the mix of both  $\text{SO}_4^{2-}$  and  $\text{Cl}^-$ , respectively, regardless of the [anion]/[Si] ratios. Table 4 summarizes the statistical metrics for each group. Undoped NBS-28 has a mean  $\delta^{30}\text{Si}$  value of  $-0.01 \pm 0.09\text{‰}$  (2SD,  $n = 97$ ), while the mean for the chloride-doped group is similar with a  $\delta^{30}\text{Si}$  of  $0.00 \pm 0.09\text{‰}$  (2SD,  $n = 48$ ), confirming there is no influence of chloride on the accuracy and precision of Si isotope measurements within our analytical uncertainty. The sulfate and sulfate plus chloride doped groups exhibit the same mean  $\delta^{30}\text{Si}$  value of  $-0.06\text{‰} \pm 0.10\text{‰}$  (2SD,  $n = 48$ ) and  $-0.06\text{‰} \pm 0.12\text{‰}$  (2SD,  $n = 74$ ), respectively. This observation suggests a potential matrix effect in both groups when comparing mean values. However, it is important to note that this shift falls within our analytical uncertainty for the mean values within each group, as observed for the individual measurements ( $n = 4$ ).

To determine whether the means of the four groups are different, we first tested the normal distribution of the groups using a Shapiro-Wilk test with a 95% confidence level. Once we confirmed that all four groups have a normal distribution, we used a *t*-test to compare the arithmetic means of the groups. The *t*-test was conducted with a 95% confidence level to test the null hypothesis, which assumes that two independent groups have identical average values for  $\delta^{30}\text{Si}$ . A *p*-value greater than 0.05 indicates that we do not have sufficient evidence to



conclude that the two means are different, while a  $p$ -value smaller than 0.05 suggests that the groups do not come from the same population and have different means. Table 4 presents the results of the  $t$ -test for the 6 possible combinations of groups. The tests conducted between undoped NBS-28 and  $\text{Cl}^-$ -doped NBS-28, as well as between  $\text{SO}_4^{2-}$ -doped and  $\text{SO}_4^{2-}$  and  $\text{Cl}^-$  doped groups, show that we do not have enough evidence to reject the null hypothesis concluding that these groups have the same mean. However, the results of the remaining tests indicate that we have enough evidence to reject the null hypothesis and conclude that undoped NBS-28 and the chloride doped groups have different means than the  $\text{SO}_4^{2-}$  doped and  $\text{SO}_4^{2-}$  and  $\text{Cl}^-$  doped groups, suggesting that they come from different populations.

Although the statistical approach revealed a shift in  $\delta^{30}\text{Si}$  of  $-0.06\text{‰}$  produced by sulfate and a mixture of sulfate and chloride contamination, this shift is substantially smaller than those reported by previous authors with values of  $+1.4\text{‰}$ ,<sup>8</sup>  $+0.28\text{‰}$ <sup>10</sup> and  $+1.04\text{‰}$ .<sup>9</sup> Moreover, considering the analytical uncertainties associated with Si isotope measurements by MC-ICP-MS, the shift in  $\delta^{30}\text{Si}$  of  $-0.06\text{‰}$  for both groups (sulfate only and sulfate + chloride) fall within errors of the undoped NBS-28, whose  $\delta^{30}\text{Si} = -0.01 \pm 0.09\text{‰}$  (2SD), as well as within the long-term reproducibility of  $\pm 0.11\text{‰}$  (2SD) obtained for the BHVO-2 standard. Consequently, we concluded that despite observing a matrix effect ( $-0.06\text{‰}$ ) produced by sulfate, chloride, or a mix of both anions, this effect is not distinguishable given our current measurement uncertainties.

### Dissolved organic carbon matrix effect

To investigate the impact of the DOC on Si isotope measurements, we analyzed natural water samples including groundwater, soil solution and stream water from three distinct catchments (see Table 2). The samples display a range of  $[\text{DOC}]/[\text{Si}]$  ratios, from 0.08 to 5.16. To identify any shift induced by the

DOC, we measured the  $\delta^{30}\text{Si}$  for each sample twice, in samples for which we applied the UV photolysis treatment described in the Method section, and in samples that were not treated. The UV photolysis was conducted before the samples were processed through ion chromatography procedure. We refer to samples that underwent UV treatment as “treated”, and the others as “untreated”.

Our dataset shows no significant difference between treated and untreated samples, with most data plotting on a 1 : 1 line (Fig. 4a and ESI Table B†). The only two samples that deviate significantly from the 1 : 1 line come from the Naizin-Kerdivy catchment and correspond to the ones with the highest  $[\text{DOC}]/[\text{Si}]$  ratios (of 4 and 5.8, Fig. 4b). The difference between the treated and untreated  $\delta^{30}\text{Si}$  value is of 0.09 and 0.10‰, respectively. As already mentioned, this limited offset is only observed in the samples from Naizin-Kerdivy catchment and cannot be only attributed to the  $[\text{DOC}]/[\text{Si}]$  ratio. In fact, one sample from the Strengbach catchment shows a high  $[\text{DOC}]/[\text{Si}]$  ratio of 5.16 but with no associated difference between treated and untreated samples. We suggest that the offset seen for the two samples from Naizin-Kerdivy catchment is related to the type of DOC present in this catchment, and not the amount of DOC. The main constituents of natural waters are humic substances, which can be classified into humic acids and fulvic acids. Together, these substances constitute approximately 60% of the total dissolved organic carbon.<sup>23</sup> Humic substances are complex molecules, and their precise structures remain unidentified.<sup>24</sup> Consequently, predicting the behavior of dissolved organic carbon during ion transmission becomes challenging due to the diverse compounds that may be present in various sample types.

Although no significant matrix effect was observed due to the presence of organic carbon, Liu *et al.*<sup>25</sup> reported that when samples are introduced into the plasma in an organic-solvent matrix or water-organic solvent mixture matrix, the resulting

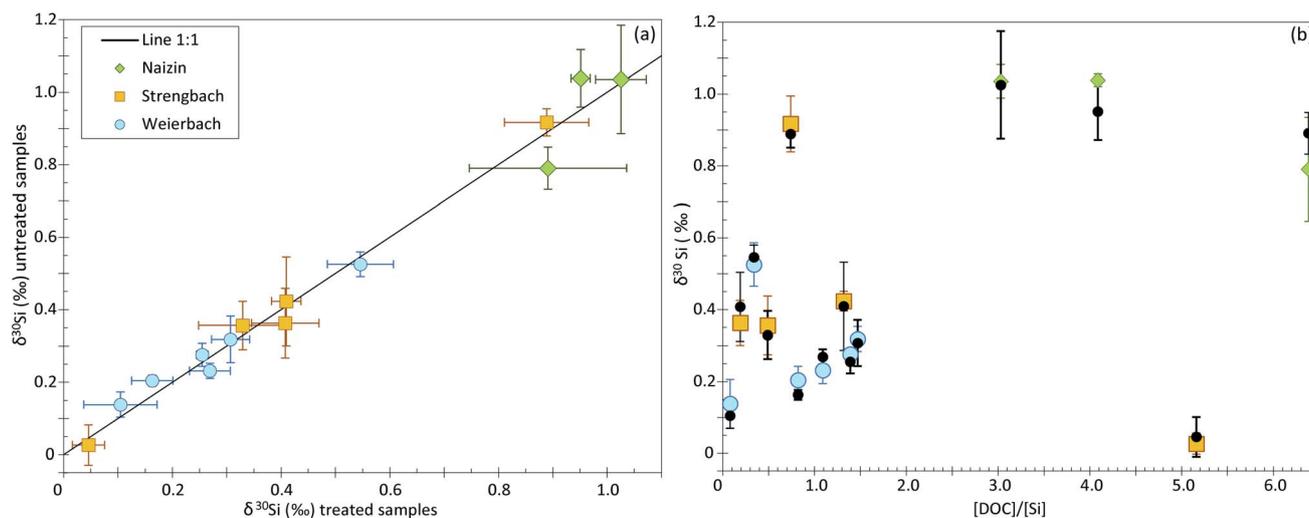


Fig. 4 (a)  $\delta^{30}\text{Si}$  values of untreated samples against that of the treated samples. Green diamonds, orange squares and blue dots represent treated samples of Naizin-Kerdivy, Strengbach and the experimental catchment of the Weierbach, respectively. (b)  $\delta^{30}\text{Si}$  values for the UV photolysis-treated and untreated samples in function of their  $[\text{DOC}]/[\text{Si}]$  ratios. Black dots represent the value of untreated samples.



organic plasma contracts and narrows along the axial and possibly along radial directions (approx. 20–30% decrease in plasma volume). Consequently, the plasma becomes more concentrated, with a higher ion density and, therefore, a greater number of ions are sampled into the interface orifice.<sup>25</sup> This may cause an increase in the sample concentration, leading to a concentration mismatch between the unknown samples and the bracketing standard resulting in inaccurate isotope measurements. To avoid potential matrix effects, we recommend using the UV photolysis method or photo-ozonolysis to remove any DOC from samples, especially for soil solutions and rivers, as proposed by Hughes *et al.*<sup>10</sup> Moreover, beyond the accurate and precise determination of the isotopic ratios, introducing high concentrations of DOC into the MC-ICP-MS is not recommended, as it may cause clogging of the nebulizer and may form deposits on the cones.

### What can cause matrix effects?

Sample matrix-based interferences are produced by the suppression or enhancement of the analyte signal compared to what is expected for the same analyte concentration in a matrix-free solution. Various factors can influence the transmission of ions from the plasma into the mass spectrometer, including the introduction system setup, the matrix of the sample solution, and the operating parameters of the instrument.

The different introduction setups appear to be the most plausible explanation for the matrix effect observed by Van Den Boorn *et al.*,<sup>8</sup> Hughes *et al.*<sup>10</sup> and Chen *et al.*,<sup>9</sup> who all measured Si isotope compositions in dry plasma using a Cetac Aridus introduction system. While the use of a desolvating system (dry plasma) offers the advantage of increasing the sensibility, it is also more sensitive to the presence of matrix and leads to a less stable signal.<sup>21</sup> Oelze *et al.*<sup>11</sup> examined the influence of anions on matrix effects in dry plasma using an ESI Apex Q introduction system and did not observe any significant shift in  $\delta^{30}\text{Si}$  values (for SSB and SSB + Mg correction). Hence, a possibility is that the desolvation membrane (present on a Cetac Aridus but absent on an Apex Q introduction system) might be responsible for increasing the matrix effects, however this should be tested. Nevertheless, Georg *et al.*<sup>5</sup> did not observe any mass bias caused by the presence of  $\text{SO}_4^{2-}$  or  $\text{NO}_3^-$ , despite using a Cetac Aridus introduction system. To explain these contrasting results, Van Den Boorn *et al.*<sup>8</sup> suggested that the difference in sample solution-medium (0.1 N HCl *vs.* 0.25 N  $\text{HNO}_3$ ) could be a contributing factor. However, the tests conducted by Van Den Boorn *et al.*<sup>8</sup> with  $[\text{SO}_4^{2-}]/[\text{Si}] = 0.4$  in HCl revealed that while 0.1 N HCl reduces the bias by approximately 1.5 times compare to 0.25 N  $\text{HNO}_3$  (+1.3‰), a significant shift of +0.8‰ persisted. Therefore, the different matrix does not appear to be entirely responsible for the significant offset caused by sulfate contamination. Our runs were performed in a 0.2 N  $\text{HNO}_3$  matrix, and we observed no shift.

Variations in instrumental parameters such as carrier flow rate, sampling depth in the plasma and ion optic settings could also be a potential explanation for the discrepancy reported between the different studies using a Cetac Aridus introduction

system. Fontaine *et al.*<sup>26</sup> evaluated the matrix effect caused by holmium (Ho) in determining the  $^{146}\text{Nd}/^{144}\text{Nd}$  ratios using a Cetac Aridus introduction system. They reported that when increasing Ho concentration in the matrix up to a factor of 6, the mass bias variation induced can be reduced increasing carrier gas flow from 1.076 to 1.131 L  $\text{min}^{-1}$ . Therefore, if the discrepancy is indeed due to instrumental parameters, matrix effects could be mitigated by optimizing the instrument parameters while measuring a reference material (such as BHVO-2, Diatomite or Big Batch) doped with a high and known amount of  $\text{SO}_4^{2-}$ . This approach can help ensure precise and accurate Si isotope measurements. Van Den Boorn *et al.*<sup>8</sup> and Chen *et al.*<sup>9</sup> also observed an increase up to 60% in the beam intensity in the solutions with  $[\text{SO}_4^{2-}]/[\text{Si}] > 0.2$  with an offset on  $\delta^{30}\text{Si}$ . Van Den Boorn *et al.*<sup>8</sup> attributed this intensity increase to either the ionization efficiency of silicon in the plasma, or the transport efficiency in the sample introduction system or in the mass spectrometer. They suggest that monitoring changes in intensity can be valuable indicator to identify any inaccurate measurements caused by  $\text{SO}_4^{2-}$  and/or DOC contamination. We specifically examined the intensity in the samples that exhibited the largest deviations among all the doping tests, but we observed no intensity increase.

Finally, another factor that could explain the discrepancy in matrix effects observed by different groups using a Cetac Aridus introduction system is the absolute concentration of anions introduced into the plasma, rather than the  $[\text{anion}]/[\text{Si}]$  ratio. Tan *et al.*<sup>27</sup> demonstrated that matrix effects in ICP-MS are more dependent on the absolute concentration of the matrix element rather than on the relative concentration of matrix to analyte. Thus, dilutions can be employed to minimize matrix effects. In fact, Van Den Boorn *et al.*<sup>8</sup> measured Si isotope compositions at higher Si concentrations, ranging from 2 to 5 ppm, compared to Georg *et al.*,<sup>5</sup> Oelze *et al.*<sup>11</sup> and this study, who measured at concentrations of 0.6 ppm, 0.6 ppm and 1 ppm respectively. Indeed, some preliminary tests conducted at IPGP show that doping NBS-28 solution with sulfur standard but with much higher Si and sulfur concentrations (20 ppm and 0.2–10 ppm, respectively), an offset up to +0.14‰ in  $\delta^{30}\text{Si}$  values was observed when  $[\text{S}]/[\text{Si}] > 0.5$  (H. Sun, personal communication). In this context, dilution during dry plasma measurements could potentially mitigate the observed matrix effects, especially if the total amount of anions is a crucial factor influencing these effects. However, further investigations are required to thoroughly assess the impact of dilution on reducing matrix effects in dry plasma.

Based on our analyses, we concluded that the discrepancy amongst studies can be primarily attributed to the use of desolvating sample introduction systems. Meanwhile, the influence of other operating parameters and the absolute quantity of sulfates introduced into the plasma seem to play a secondary role.

## Conclusions

We did not observe any significant offset in  $\delta^{30}\text{Si}$  values outside the range of our analytical precision ( $\pm 0.09\%$ , 2SD) induced by



## Technical Note

the presence of chloride, sulfate or dissolved organic carbon in the matrix, across a range of  $[Cl^-]/[Si] = 0.09$  to  $5.65$ ,  $[SO_4^{2-}]/[Si] = 0.09$  to  $5.65$  and  $[DOC]/[Si] = 0.08$  to  $6.38$ . Statistical tests reveal a mean shift of  $-0.06\%$  in solutions doped with  $SO_4^{2-}$  and a mixture of  $SO_4^{2-}$  and  $Cl^-$ , indicating the presence of matrix effects. However, this shift falls within analytical uncertainty, considering the current precision in Si isotopes measurements by MC-ICP-MS. Although the offset due to DOC contamination was less than  $0.10\%$  and fell within the range of analytical uncertainty, we recommend removal of DOC from samples. We have presented an easy and rapid methodology to remove organic matter from water samples and ensure accurate and precise Si isotope measurements. Our results indicate that precise and accurate measurements ( $<0.11\%$ , 2SD) can be attained for stable Si isotope ratios by MC-ICP-MS in wet plasma, with a larger tolerance to sample based-matrix effect induced by anion contamination compared to dry plasma.

## Author contributions

Sofía López-Urzúa: conceptualization, data curation, formal analysis, methodology, investigation, writing – original draft. Tu-Han Luu: Writing – review & editing. Louis Derry: funding acquisition, project administration, resources, writing – review & editing.

## Conflicts of interest

There are no conflicts to declare.

## Acknowledgements

This study was financially supported by Agence Nationale de la Recherche (ANR) through the “Investissements d'avenir” program under the project CZTOP (n 725 ANR-17-MPGA726 0009). We greatly thank Dimitri Rigoussen for technical support with MC-ICP-MS analyses and Pierre Burckel for the measurement of Si concentrations by ICP-MS Agilent 7900. We also thank Mark Brzezinski and Janice Jones for kindly providing the Diatomite and Big Batch standards. We are grateful for the thoughtful and constructive comments by two anonymous reviewers.

## References

- 1 J. H. Reynolds and J. Verhoogen, Natural variations in the isotopic constitution of silicon, *Geochim. Cosmochim. Acta*, 1953, **3**(5), 224–234.
- 2 C. L. De La Rocha, Measurement of silicon stable isotope natural abundances via multicollector inductively coupled plasma mass spectrometry (MC-ICP-MS), *Geochem., Geophys., Geosyst.*, 2002, **3**(8), 1–8.
- 3 E. Engström, I. Rodushkin, D. C. Baxter and B. Öhlander, Chromatographic Purification for the Determination of Dissolved Silicon Isotopic Compositions in Natural Waters by High-Resolution Multicollector Inductively Coupled Plasma Mass Spectrometry, *Anal. Chem.*, 2006, **78**(1), 250–257.
- 4 T. Ding, D. Wan, C. Wang and F. Zhang, Silicon isotope compositions of dissolved silicon and suspended matter in the Yangtze River, China, *Geochim. Cosmochim. Acta*, 2004, **68**(2), 205–216.
- 5 R. B. Georg, B. C. Reynolds, M. Frank and A. N. Halliday, New sample preparation techniques for the determination of Si isotopic compositions using MC-ICPMS, *Chem. Geol.*, 2006, **235**(1–2), 95–104.
- 6 S. H. J. M. Van Den Boorn, P. Z. Vroon, C. C. Van Belle, B. Van Der Wagt, J. Schwieters and M. J. Van Bergen, Determination of silicon isotope ratios in silicate materials by high-resolution MC-ICP-MS using a sodium hydroxide sample digestion method, *J. Anal. At. Spectrom.*, 2006, **21**(8), 734.
- 7 J. W. Olesik, Inductively Coupled Plasma Mass Spectrometers, in *Treatise on Geochemistry*, Elsevier, 2014, pp. 309–336.
- 8 S. H. J. M. Van Den Boorn, P. Z. Vroon and M. J. Van Bergen, Sulfur-induced offsets in MC-ICP-MS silicon-isotope measurements, *J. Anal. At. Spectrom.*, 2009, **24**(8), 1111.
- 9 X. Chen, T. J. Lapen and H. S. Chafetz, Accurate and Precise Silicon Isotope Analysis of Sulfur- and Iron-Rich Samples by MC - ICP - MS, *Geostand. Geoanal. Res.*, 2017, **41**(3), 427–435.
- 10 H. J. Hughes, C. Delvigne, M. Korntheuer, J. De Jong, L. André and D. Cardinal, Controlling the mass bias introduced by anionic and organic matrices in silicon isotopic measurements by MC-ICP-MS, *J. Anal. At. Spectrom.*, 2011, **26**(9), 1892.
- 11 M. Oelze, J. A. Schuessler and F. Von Blanckenburg, Mass bias stabilization by Mg doping for Si stable isotope analysis by MC-ICP-MS, *J. Anal. At. Spectrom.*, 2016, **31**(10), 2094–2100.
- 12 F. Gaspard, S. Opfergelt, C. Dessert, V. Robert, Y. Ameijeiras-Mariño and P. Delmelle, Imprint of chemical weathering and hydrothermalism on the Ge/Si ratio and Si isotope composition of rivers in a volcanic tropical island, Basse-Terre, Guadeloupe (French West Indies), *Chem. Geol.*, 2021, **577**, 120283.
- 13 C. O'Connor, B. L. Sharp and P. Evans, On-line additions of aqueous standards for calibration of laser ablation inductively coupled plasma mass spectrometry: theory and comparison of wet and dry plasma conditions, *J. Anal. At. Spectrom.*, 2006, **21**(6), 556.
- 14 C. Agatemor and D. Beauchemin, Matrix effects in inductively coupled plasma mass spectrometry: A review, *Anal. Chim. Acta*, 2011, **706**(1), 66–83.
- 15 C. Hissler, N. Martínez-Carreras, F. Barnich, L. Gourdol, J. F. Iffly, J. Juilleret, *et al.*, The Weierbach experimental catchment in Luxembourg: A decade of critical zone monitoring in a temperate forest - from hydrological investigations to ecohydrological perspectives, *Hydrol. Processes*, 2021, **35**(5), e14140.
- 16 M. C. Pierret, S. Cotel, P. Ackerer, E. Beaulieu, S. Benarioumlil, M. Boucher, *et al.*, The Strengbach Catchment: A Multidisciplinary Environmental Sentry for 30 Years, *Vadose Zone J.*, 2018, **17**(1), 1.



- 17 O. Fovet, L. Ruiz, G. Gruau, N. Akkal, L. Aquilina, S. Busnot, *et al.*, AgrHyS: An Observatory of Response Times in Agro-Hydro Systems, *Vadose Zone J.*, 2018, **17**(1), 1–16.
- 18 D. Cardinal, L. Y. Alleman, J. De Jong, K. Ziegler and L. André, Isotopic composition of silicon measured by multicollector plasma source mass spectrometry in dry plasma mode, *J. Anal. At. Spectrom.*, 2003, **18**(3), 213–218.
- 19 B. C. Reynolds, J. Aggarwal, L. André, D. Baxter, C. Beucher, M. A. Brzezinski, *et al.*, An inter-laboratory comparison of Si isotope reference materials, *J. Anal. At. Spectrom.*, 2007, **22**(5), 561–568.
- 20 K. P. Jochum, U. Nohl, K. Herwig, E. Lammel, B. Stoll and A. W. Hofmann, GeoReM: A New Geochemical Database for Reference Materials and Isotopic Standards, *Geostand. Geoanal. Res.*, 2005, **29**(3), 333–338.
- 21 C. Delvigne, A. Guihou, J. A. Schuessler, P. Savage, F. Poitrasson, S. Fischer, *et al.*, Silicon Isotope Analyses of Soil and Plant Reference Materials: An Inter-Comparison of Seven Laboratories, *Geostand. Geoanal. Res.*, 2021, **45**(3), 525–538.
- 22 P. Vermeesch, IsoplotR: A free and open toolbox for geochronology, *Geosci. Front.*, 2018, **9**(5), 1479–1493.
- 23 E. M. Thurman. Amount of Organic Carbon in Natural Waters, in *Organic Geochemistry of Natural Waters*, Springer Netherlands, Dordrecht, 1985, pp. 7–65.
- 24 W. M. White, Organic geochemistry, the carbon cycle, and climate, in *Geochemistry*, Wiley-Blackwell, Chichester, West Sussex: Hoboken, NJ, 2013, p. 1.
- 25 S. Liu, Z. Han, X. Kong, J. Zhang, Z. Lv and G. Yuan, Organic matrix effects in inductively coupled plasma mass spectrometry: a tutorial review, *Appl. Spectrosc. Rev.*, 2022, **57**(6), 461–489.
- 26 G. H. Fontaine, B. Hattendorf, B. Bourdon and D. Günther, Effects of operating conditions and matrix on mass bias in MC-ICPMS, *J. Anal. At. Spectrom.*, 2009, **24**(5), 637.
- 27 S. H. Tan and G. Horlick, Matrix-effect observations in inductively coupled plasma mass spectrometry, *J. Anal. At. Spectrom.*, 1987, **2**(8), 745.

