


JAAS

Journal of Analytical Atomic Spectrometry

rsc.li/jaas

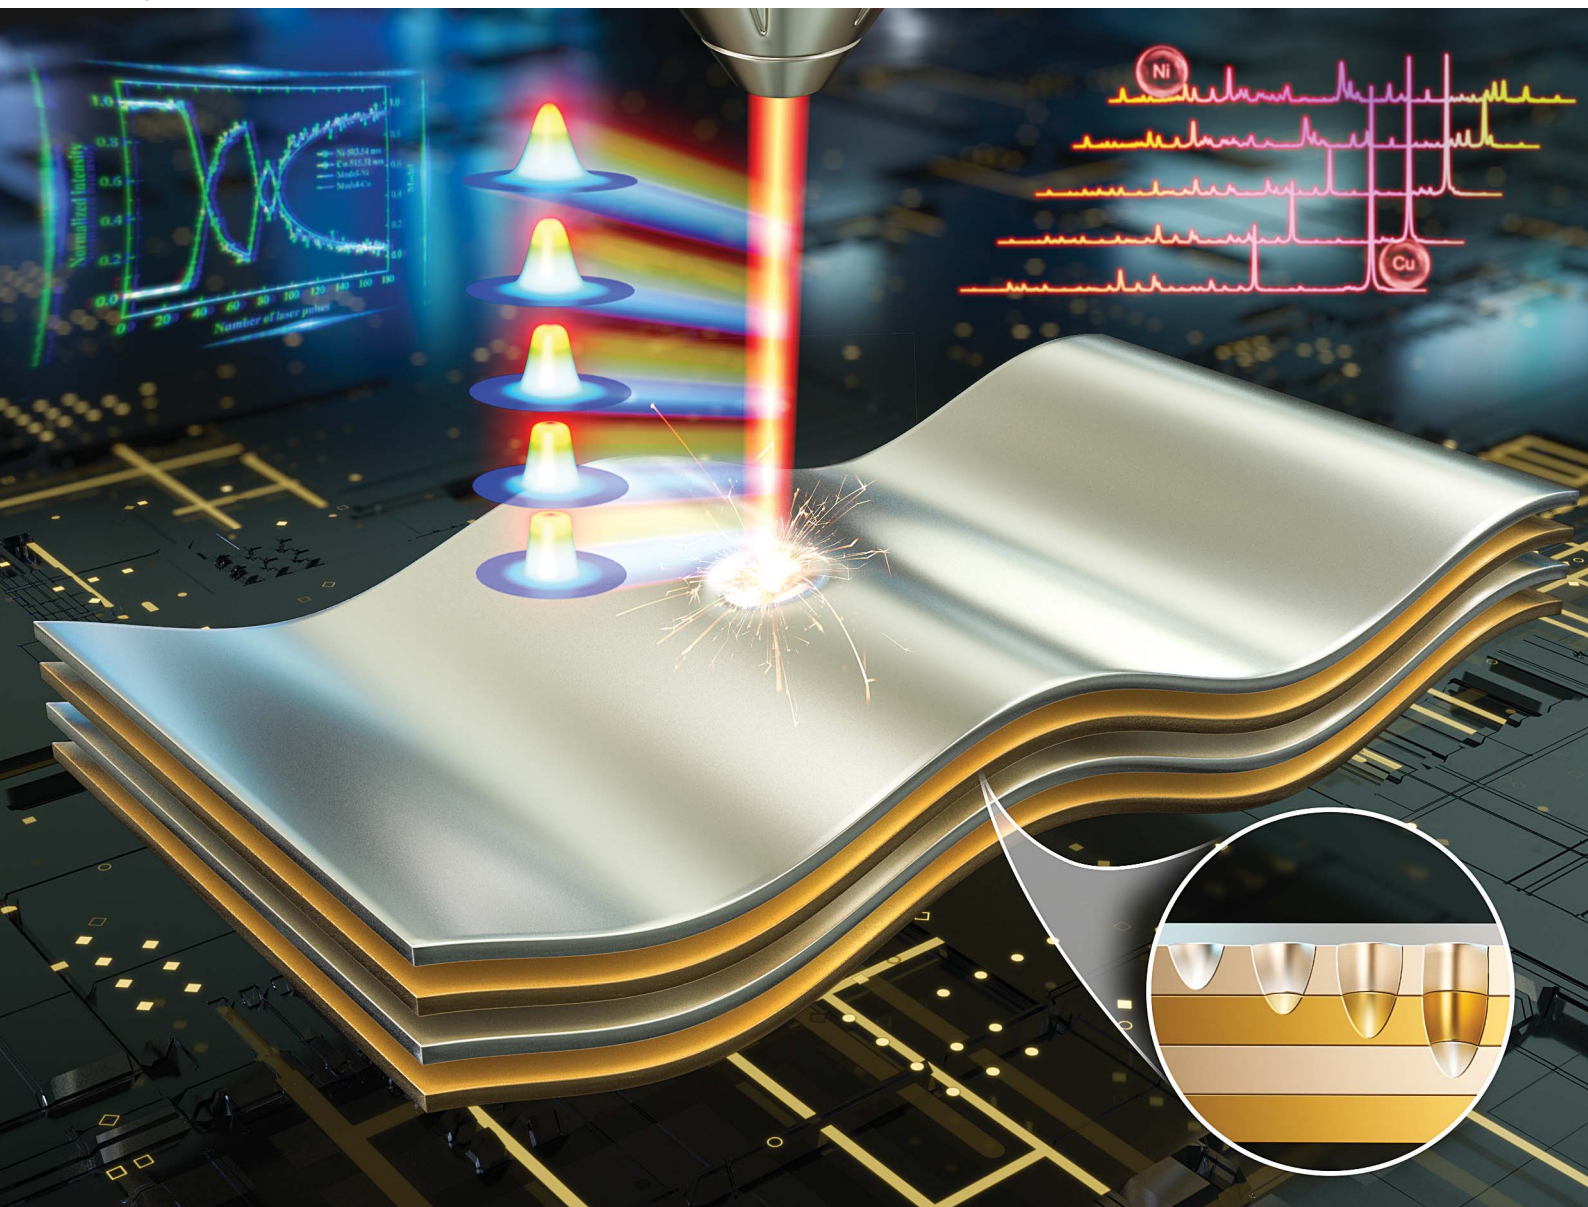

ISSN 0267-9477

PAPER

Cong Li *et al.*

Study of the layer thickness of multilayer sample by the LIBS method based on ablation rate correction