

Analyst

Accepted Manuscript



This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

Selective vancomycin detection using optical fibre long period gratings functionalised with molecularly imprinted polymer nanoparticles

Sergiy Korposh^{1*}, Iva Chianella², Antonio Guerreiro², Sarah Caygill², Sergey Piletsky², Stephen W. James¹, Ralph P. Tatam¹

¹Department of Engineering Photonics, School of Engineering, Cranfield University, Cranfield, Bedfordshire, MK43 0AL, UK

²Cranfield Health, Cranfield University, Cranfield, Bedfordshire, MK43 0AL, UK

*Corresponding author: s.korposh@cranfield.ac.uk


Abstract

An optical fibre long period grating (LPG) sensor modified with molecularly imprinted polymer nanoparticles (nanoMIPs) for the specific detection of antibiotics is presented. The operation of the sensor is based on the measurement of changes in refractive index induced by the interaction of nanoMIPs deposited onto the cladding of the LPG with free vancomycin (VA). The binding of nanoMIPs to vancomycin was characterised by a binding constant of $4.3 \pm 0.1 \times 10^{-8}$ M. The lowest concentration of analyte measured by the fibre sensor was 10 nM. In addition, the sensor exhibited selectivity, as much smaller responses were obtained for high concentrations (~ 700 μ M) of other commonly prescribed antibiotics such as amoxicillin, bleomycin and gentamicin. In addition, the response of the sensor was characterised in a complex matrix, porcine plasma, spiked with 10 μ M of VA.

1. Introduction

Fibre optic devices coated with functional nanomaterials that exhibit changes in optical properties upon exposure to targeted chemical species have emerged as a promising platform for the development of bio- and chemical sensors^{1, 2}. The characteristics of such sensors, such as sensitivity, selectivity and response/recovery time, depend strongly upon the performance capabilities and properties of the functional layer. Research in the field of fibre optic chemical sensors has focused recently on the development of new functional coatings. The functional materials should be transparent in the appropriate spectral range, change their optical properties under the influence of the specific chemical species, have fast, ideally reversible response with a wide dynamic range, be readily immobilized onto glass/quartz/plastic fibre, and be cheap to manufacture. In this regard, molecularly imprinted polymers (MIPs) provide a universal platform for the creation of artificial receptors that can be well controlled and tailored.

Molecular imprinting is one of the most promising approaches for achieving specific molecular recognition. The technique is versatile, as any compound with functional groups can, in principle, be imprinted in different porogens (either water or organic solvents). The basic concept of molecular imprinting is based on the creation of imprints of the template compound (i.e. chemical molecules or biological species that needs to be detected – analytes) in a polymeric matrix, achieved by its incorporation during the polymerization step. Molecular imprinting is achieved in three steps, the first being the complex formation of the template with selected functional monomers, followed by a polymerization step for creation of a matrix that fixes the monomers in the right position to interact with the analyte and with the final step being the removal of the template to leave behind cavities specific for the template, Scheme1.

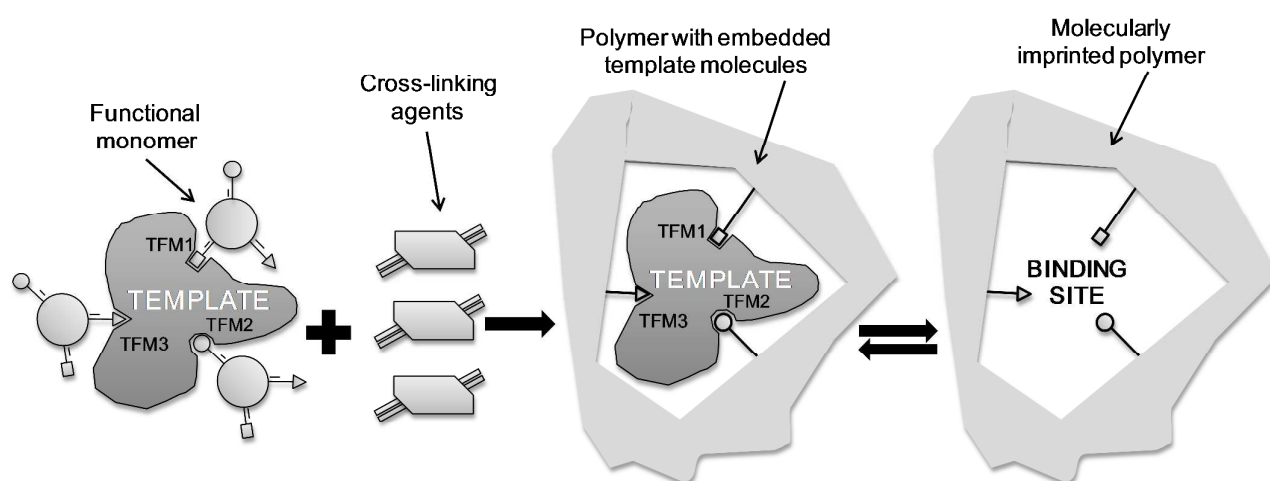

Scheme 1. Schematic illustration of the molecular imprinting procedure³.

Although MIPs have already been identified as stable and low cost mimics of receptors or enzymes for sensing applications^{4, 5, 6, 7}, they are also perceived to have several shortcomings. Among these are the heterogeneous distributions of binding sites, which can produce high levels of non-specific binding and have complex protocols for integration with sensors, which can affect the reproducibility and hence increase the variability between measurements. Some of these issues can be resolved by the use of MIP nanoparticles (nanoMIPs) in standard protocols developed for the immobilisation of antibodies. The particles used here were produced by a solid-phase synthesis approach using a computer-controlled reactor. Such MIP nanoparticles have been shown to have pseudo-monoclonal binding properties, uniform binding sites and high affinity for the target used as the template^{8, 9}. Recently, such MIP nanoparticles were used for the detection of vancomycin in a novel assay based on direct replacement of antibodies¹⁰. The assay was capable of measuring vancomycin in buffer and in blood plasma within the range of 0.001–70 nM with a detection limit of 0.0025 nM (2.5 pM).

1 In this work, nanoparticles produced following the protocol described in [10] were deposited onto
2 an optical fibre long period grating (LPG) with the aim of developing a low cost, highly sensitive and
3 selective vancomycin sensor. Vancomycin is a glycopeptide antibiotic derived from *Amycolatopsis*
4 *orientalis*¹¹. The mode of action of vancomycin consists of the inhibition of cell wall biosynthesis and
5 alteration of the permeability of the bacterial cell membrane. Vancomycin has been used to treat various
6 serious gram-positive infections. It is a powerful antibiotic, which in high doses can be toxic to the ears
7 and kidneys, whilst at low doses can cause hypersensitivity reactions. Thus it is important to measure
8 accurately the concentration of vancomycin in blood to control its administration to patients. The
9 recommended therapeutic concentration range of vancomycin in plasma is 15-20 mg/L¹².
10 Immunoenzymatic techniques (e.g. fluorescence polarisation immunoassay (FPIA)(TDx), enzyme
11 multiplied immunoassay technique (EMIT), radioimmunoassay (RIA), turbidimetric assays) and
12 chromatographic methods are the most commonly used in clinical environments for the detection of
13 vancomycin in plasma¹³. The former, although widely used because of their simplicity and speed, lacks
14 precision, especially for the highest concentrations of the antibiotic^{14, 15}. The latter can be very precise,
15 but the techniques are time consuming and require expensive instruments and highly skilled operators.
16 Therefore there is a need to develop reliable, fast, cheap and easy to use sensors for clinical measurements
17 of vancomycin and antibiotics in general.

18 Regarding the sensor platform, a long period grating (LPG) is a periodic modulation of the
19 refractive index (RI) of the core of an optical fibre that results in the coupling of light between core and
20 cladding modes. Its combination with nanomaterials provides a prospect for the fabrication of high
21 sensitivity sensors offering specific binding to targeted chemical species^{16, 17}. Recently, we have
22 demonstrated the use of optical fibre LPG sensors modified with different functional coatings for the
23 detection of ammonia¹⁸ and aromatic carboxylic acids¹⁹.

24 The coupling between core and cladding modes occurs when the phase matching condition is
25 satisfied:

$$\lambda_x = (n_{core} - n_{clad(x)})\Lambda \quad (1)$$

26 where λ_x represents the wavelength at which light is coupled to the LP_{0x} cladding mode, n_{core} is the
27 effective refractive index of the mode propagating in the core of the fibre, $n_{clad(x)}$ is the effective index of
28 the LP_{0x} cladding mode and Λ is the period of the LPG.


29 The transmission spectrum of an optical fibre containing an LPG is characterised by a series of
30 resonance bands centred at the wavelengths satisfying equation 1. The dependences of the cladding
31 modes' effective refractive indices on the surrounding refractive index are manifested as changes in the
32 central wavelengths of the resonance bands, which has been exploited as a refractive index sensor and
33 non-specific concentration sensor²⁰, and by, coating with the cladding of the optical fibre in the section
34 containing the LPG with a functional material, chemical sensors in both the liquid and gas phases^{17, 18}.

1 The combination of optical fibre based sensing platforms with MIPs has already been attempted
2 by several research groups. Previous reports have exploited surface plasmon resonance on metal coated
3 optical fibres^{21, 22} or have used a fluorescence signal²³, rather than LPGs. In all of these examples the MIP
4 layer was produced *in situ* on the fibre, making large scale production of the optical sensors more
5 challenging because of the need to control polymerization conditions to achieve high quality and
6 reproducible MIP layers. In this paper, the MIP layer was deposited onto the optical fibre by simply
7 immersing the optical fibre into a solution of soluble and easy-to-manipulate MIP nanoparticles. The
8 nanoMIPs-modified optical fibre LPG was used to measure vancomycin in a concentration range from 10
9 nM to 700 μ M, equivalent to 14 μ g/L and 1 g/L, respectively. The lower concentration was chosen with
10 the intention of assessing if this sensor was capable of measurements in dilutions of real samples, which
11 would be helpful to reduce interferences when testing biological samples like plasma. The mid-range
12 includes the recommended therapeutic concentration range, while the higher concentration was
13 investigated to assess the concentrations at which the sensor response saturates. The selectivity of the
14 sensor was tested against other commonly prescribed antibiotics such as gentamicin, amoxicillin and
15 bleomycin²⁴. In addition, to check the sensor performance in a complex biological matrix, the response to
16 vancomycin was also measured in porcine plasma spiked with the antibiotic.
17
18
19
20
21
22
23
24
25
26
27
28

29 **2. Experimental section**

30 **2.1 Materials**

31
32
33 N -isopropylacrylamide (NIPAm), acrylic acid (AA), *N, N'* methylene-bis-acrylamide (BIS), *N*-tert-
34 butylacrylamide (TBAm), ammonium persulfate (APS), tetramethylethylenediamine (TEMED), 3-
35 aminopropyltrimethyloxysilane (APTMS), glutaraldehyde (GA), ethanolamine, phosphate buffered saline
36 (PBS), methanol, ethanol, toluene and acetone were purchased from Sigma-Aldrich, UK. The antibiotics
37 vancomycin (VA), amoxicillin, bleomycin sulphate salt, gentamicin sulphate salt (Scheme 1) were also
38 from Sigma-Aldrich. *N*-(3-aminopropyl)methacrylamide hydrochloride (APMA) was from Polysciences
39 Europe GmbH, Germany. All the chemicals were of analytical grade, and used without further
40 purification. Double-distilled ultrapure water (Millipore, UK) was used for the experiments. Phosphate
41 buffered saline (PBS) was prepared as directed from PBS buffer tablets (Sigma- Aldrich, Gillingham,
42 UK) and comprised phosphate buffer (0.01 M), potassium chloride (0.0027 M) and sodium chloride
43 (0.137 M), pH 7.4, at 25 ° C. Where PBS, pH 7.2, was used, the pH was adjusted by the addition of HCl.
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

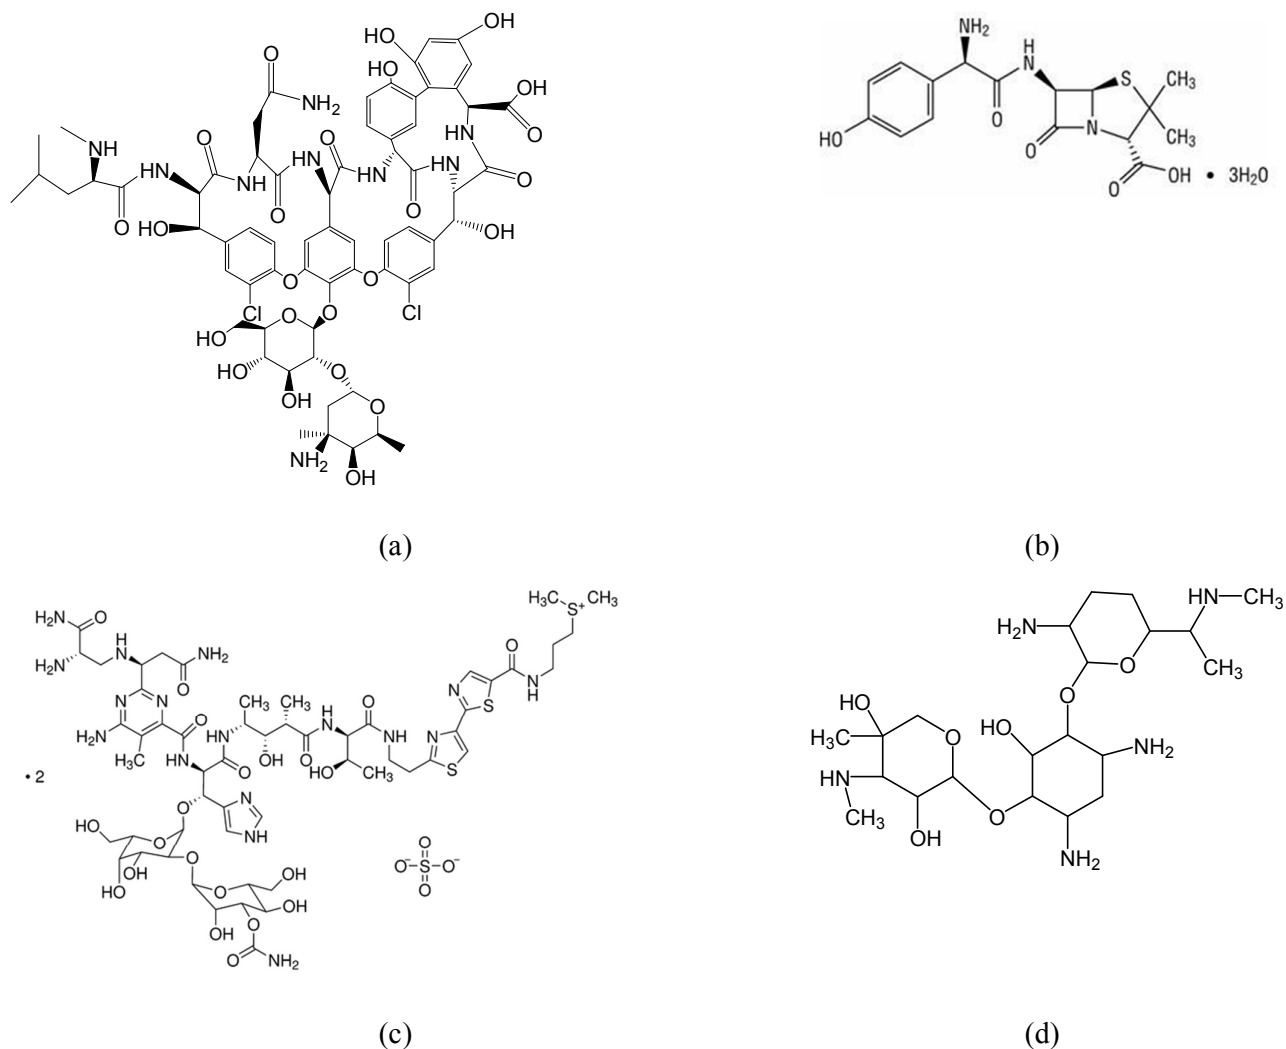

Scheme 2: Schematic illustration of the chemicals used for detection and selectivity tests: (a) vancomycin (VA); (b) amoxicillin; (c) bleomycin and (d) gentamicin.


2.2 Synthesis of MIP nanoparticles (nanoMIPs) imprinted with vancomycin

The protocol for the immobilization of vancomycin on solid supports (glass beads) has been described elsewhere⁸. An automated reactor, upgraded compared to that used previously⁸, was utilized for the synthesis of the nanoparticles. During the entire synthesis the template remains attached to the glass beads. Once the high affinity nanoparticles, formed around the template, are collected with hot washing, the template still remains attached to the solid surface and the nanoparticles collected are already ‘template free’. This is one of the major advantages of the solid-support approach in comparison with other methods used for the synthesis of nanoparticles. Regarding the details of the automated synthesis, the reactor, manufactured by HEL Ltd., (Borehamwood, UK), was designed to allow both photochemically- and chemically-initiated polymerizations. All processes were controlled with a computer, with minimal intervention from the operator. For the preparation of nanoMIPs specific for

1 vancomycin, the polymerization mixture, which was adapted from that published by Hoshino and
2 colleagues²⁵ consisted of NIPAm (39 mg), BIS (2 mg), TBAm (33 mg dissolved in 2 mL of ethanol),
3 APMA (1.15 mg) and AA (2.23 g). The mixture was dissolved in double distilled water (100 ml),
4 sonicated for 10 minutes and degassed by bubbling with nitrogen for 30 minutes. For the automated
5 synthesis of nanoMIPs, glass beads functionalized with vancomycin (60 g) were added to the reaction
6 cylinder. Using a syringe pump, an aliquot of the polymerization mixture (60 mL) was added directly into
7 the cylinder and then stirred briefly to homogenize the contents. Polymerization was initiated by the
8 addition of a solution of APS (60 mg mL⁻¹, 600 µL) and TEMED (18 µL) followed by stirring. The
9 monomer mixture was left to polymerize at ambient temperature for 1.5 hours and a brief stirring (30 s at
10 600 RPM) was applied at the end of each 30 min period. At the end, the polymerization mixture was
11 drained from the reaction vessel using a combination of suction and nitrogen purging. Subsequently,
12 washings were performed at ambient temperature by adding water (2 aliquots of 50 mL) to the cylinder.
13 The contents were stirred and the washings, containing unreacted monomers and other low affinity
14 materials, removed and discarded. Next, a further 3 aliquots of water (50 mL each) were individually
15 added to the cylinder and the temperature was raised to 60 °C. At this temperature pure fractions of
16 nanoparticles were collected. The entire process took approximately 3.5 hours. The stages of the synthesis
17 were pre-programmed into the WinISO® software such that, once started, the synthesis could be left to run
18 without the necessity for user supervision. The solution of nanoMIPs was concentrated to a final volume
19 of 100 mL by ultrafiltration on a Millipore Amicon Ultra centrifugal filter unit (30 kDa MWCO) and its
20 concentration (0.2 mg/ml) determined by weighing a freeze-dried aliquot. The size of the nanoparticles
21 measured by dynamic light scattering (DLS) using a Zetasizer Nano (Nano-S) from Malvern Instruments
22 Ltd (Malvern, UK) was around 280 nm. Prior to DLS measurements, performed at 25 °C, the solution of
23 nanoMIPs was subjected to sonication for 5 minutes.

2.3 Sensor fabrication and functionalization

41 An LPG with a length of 30 mm and a period of 111 µm was fabricated in boron–germanium co-doped
42 single mode optical fibre (Fibercore PS750) with a cut-off wavelength of 670 nm, in a point-by-point
43 fashion, side-illuminating the optical fibre by the output from a frequency-quadrupled Nd:YAG laser,
44 operating at 266 nm. The period of the LPG was chosen to ensure operation at the phase matching turning
45 point, a condition known to offer the highest sensitivity²⁶. The fibre was fixed tightly in a Teflon cell as
46 described previously¹⁵⁻¹⁸. For transmission spectra (TS) measurements, one proximal end of the fibre was
47 connected to a spectrometer (S200, Ocean Optics) and the distal end to a tungsten halogen lamp (HL-
48 2000, Ocean Optics).

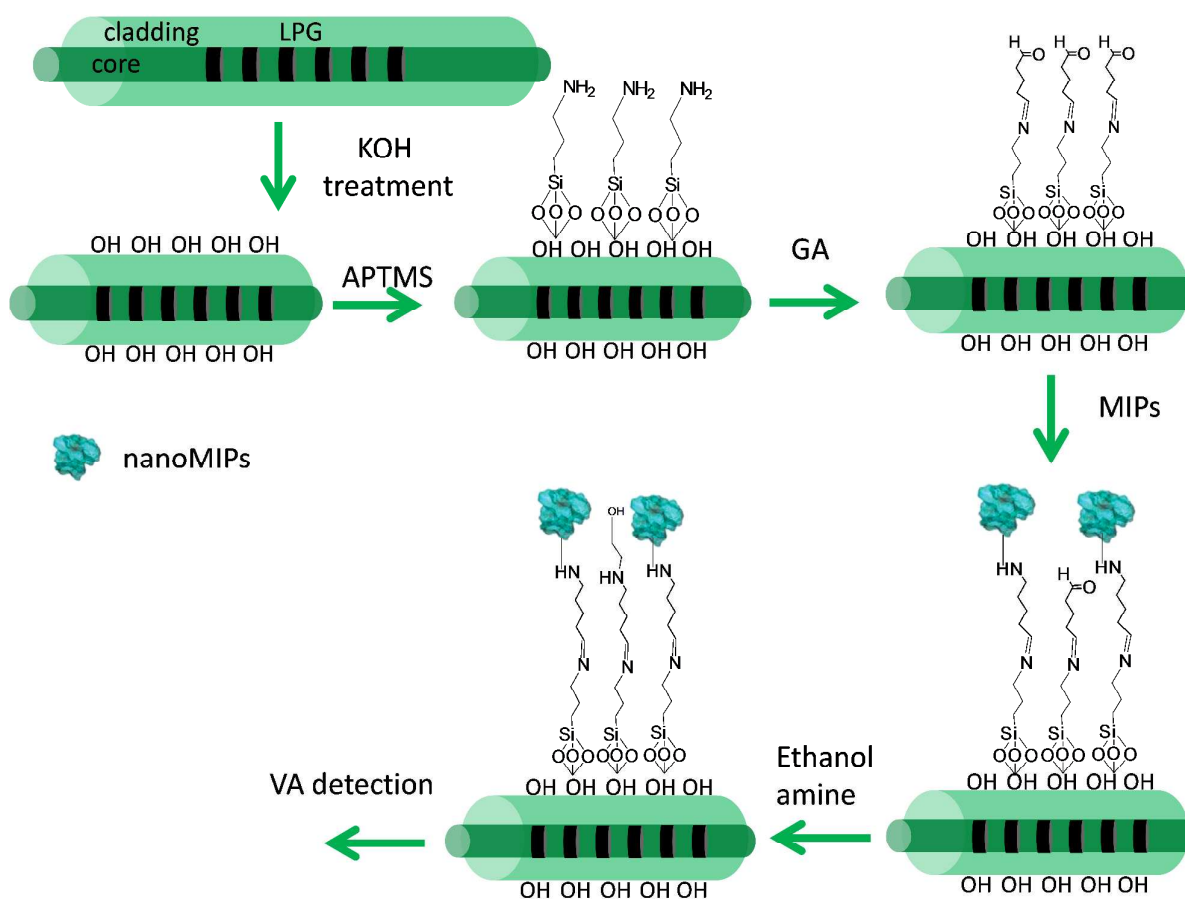

Scheme 3: Schematic illustration of the protocol used to immobilize nanoMIPs

Prior to the deposition of the nanoMIPs, the region of the optical fibre containing the LPGs was rinsed with double-distilled water and immersed into 1 wt% ethanolic KOH (ethanol/water = 3:2, v/v) for 20 min, leading to formation of hydroxyl groups on the fibre surface. The fibre was then immersed into a 2% v/v solution of APTMS in dry toluene for different time intervals to find the optimal conditions, washed with acetone and subsequently incubated in a 1% v/v solution of GA in PBS (pH 7.2) for 1 hour. The LPG fibre was then rinsed with double-distilled water and immersed into a nanoMIPs solution (0.2 mg/ml) for 2 h. After rinsing with double distilled water, the fibre was immersed for 30 minutes into an ethanolamine water solution (0.1 M), to block the remaining free carbonyl groups of GA, and following a final wash with double-distilled water, the sensor was ready to be used. A schematic representation of the nanoMIPs immobilization protocol is reported on Scheme 3. The transmission spectrum (TS) of the LPG was measured after each step of the surface treatment.

2.4 Sensitivity and selectivity tests

After the functionalization, the sensor was exposed to variable concentrations of VA by immersion into 600 μL solution for 45 min, as after this time there was no change in measured signal. This was followed by thorough rinsing with distilled water and drying by purging with dry nitrogen to remove any physically adsorbed compounds. The transmission spectrum (TS) of the LPG was measured after each exposure to analyte and interfering substances. To avoid issues with sensitivity of the LPG to the bulk refractive index, all TS measurements were conducted in air. In order to take into account the potential difference in the light source intensity between different measurements the TS were normalised by taking an automatic baseline for each measured TS using Origin 7.5 software. After each exposure, a solution of NaOH (0.1 M) was used to regenerate the sensor by removing the VA adsorbed to the nanoMIPs. The sensor selectivity was tested by exposure to other common antibiotics (amoxicillin, gentamicin and bleomycin) with a concentration of 600-700 μM . The nanoMIPs-modified LPG was also immersed into porcine plasma spiked with 10 μM of vancomycin to check the sensor performance in a complex biological matrix.

It should be noted that the effect of the non-imprinted nanoparticles was thoroughly studied in the previous work with ELISA assay¹⁰ where the imprinting effect of the nanoMIPs was clearly demonstrated and was not included in this current study.

3 Results and discussion

3.1 NanoMIPs deposition

The first step to immobilize covalently nanoMIPs onto the optical fibre involved the deposition of a thin silane film onto the hydroxyl groups on the fibre surface formed by the KOH ethanolic solution. To do this the fibre was immersed into 2% v/v solution of APTMS in dry toluene. The silane also provides the surface with the primary amino groups necessary for the subsequent immobilization steps. Figure 1 shows the TS of the LPG with grating period of 111 μm , measured in air before and after 1 hour deposition of the APTMS. It should be noted that, in order to take into account the potential difference in the intensity of the light source between different measurements (Figure S1), the TS were normalised by taking an automatic baseline for each measured TS using Origin 7.5 software. The blue shift of the linearly polarised (LP) mode LP_{018} resonance, along with the appearance of the dual resonance for the LP_{019} mode resonance, is characteristic of the response of the LPG to the deposition of a thin film onto the cladding of the fibre.


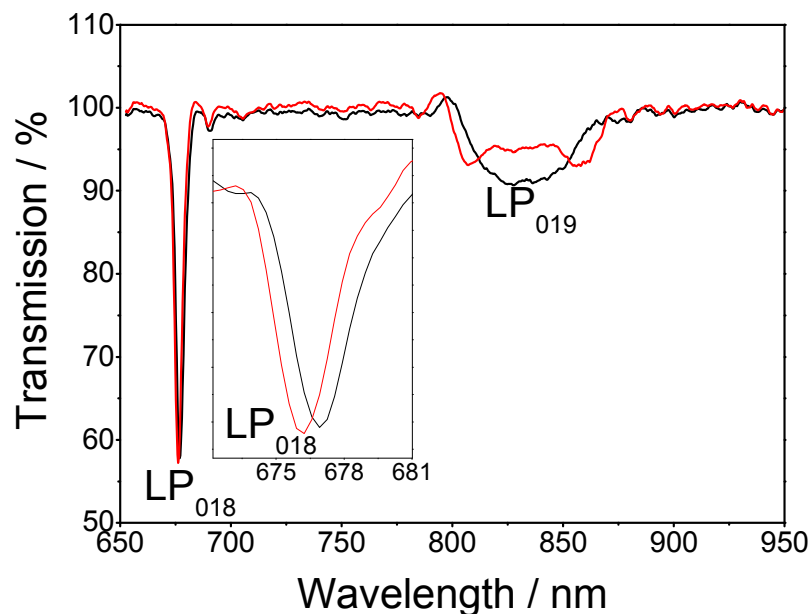



Figure 1. TS of the LPG measured in air: black line, before APTMS deposition, and red line, after APTMS deposition

Following the deposition of the silane, the fibre was immersed into a PBS solution of GA, Figures 2a and 2b. Similarly to that observed following the deposition of the APTMS film, a further blue shift of the LP_{018} resonance, and further development of the LP_{019} dual resonance bands were observed, demonstrating a successful deposition of GA *via* attachment of the carbonyl groups of GA to the amino groups of the silane. When measured in solution, the LP_{019} resonance band exhibited a significant wavelength shift during the first 15 min from the start of the GA deposition, with the response saturating at around 30 min, as shown in Figure 2a. Figure 2b shows the TS measured in air before and after GA deposition, with the changes in the spectra indicating an increase of the optical thickness of the film.

After GA deposition, the LPG was immersed into a water solution of nanoMIPs (0.2 mg/ml) for 2 hours, Figure S2. The amino groups contained in the NanoMIPs (due to the monomer APMA) create a bond with the carbonyl groups of GA. The minor change in the LP_{018} resonance band apparent after the immobilization of nanoMIPs can be explained by successful attachment of the nanoparticles to the GA surface. The final step of the MIP sensor fabrication was the blocking by ethanolamine (0.1 M) of any available carbonyl groups remaining on GA, Figure S3. A small change in the TS was observed, revealing the adsorption of the ethanolamine.

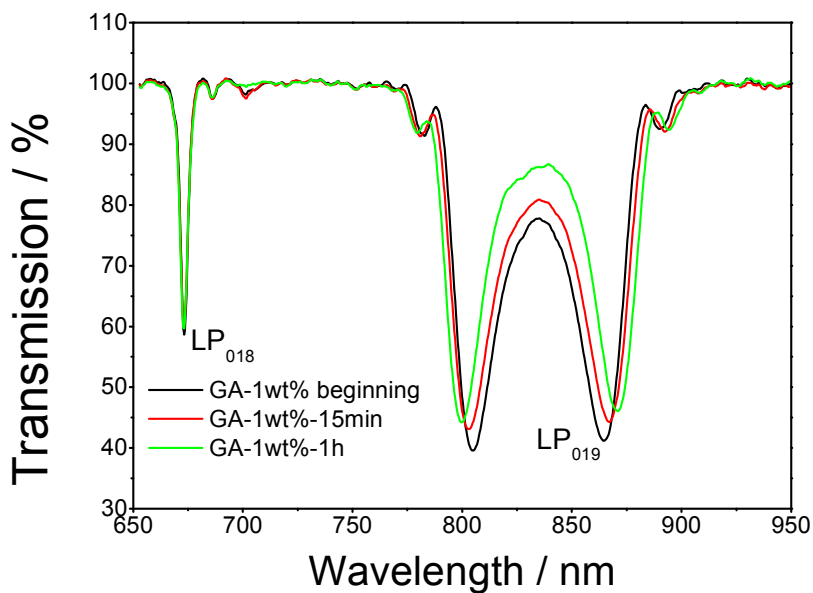

(a)

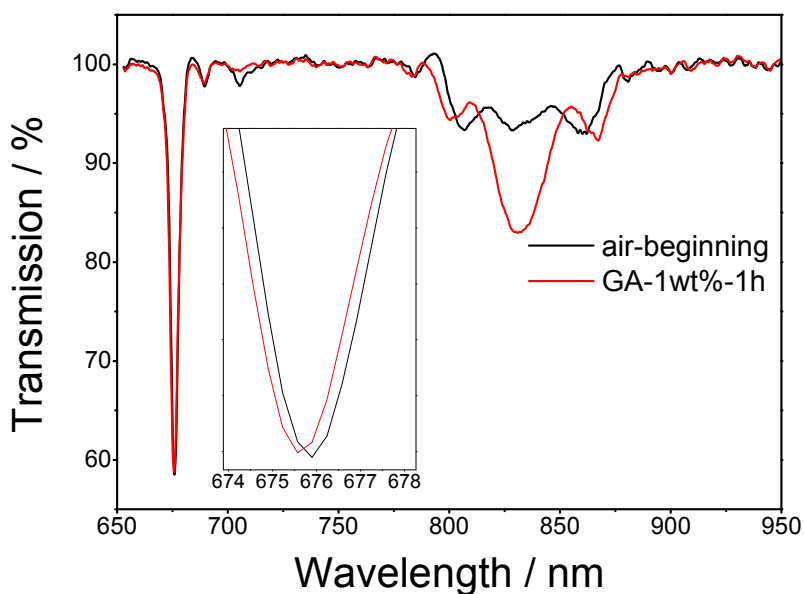


(b)


Figure 2. (a) Evolution of the TS of the APTMS-coated optical fibre LPG during the deposition of 1wt % GA, measured in solution at different interval times: black line, before GA deposition; red line, 15 min; and green line, 1 h after GA deposition; (b) TS measured in air: black line, before GA deposition, and red line, after GA deposition;

3.2 Vancomycin detection

After the immobilization of the nanoMIPs and blocking with ethanolamine, the LPG was exposed to increasing concentrations of VA solution. Each concentration was incubated for 45 minutes (Figure 3a) as, after this time, the signal was saturated, Figure S4. It should be noted, however, that these data cannot be directly used to assess amount that was bound, as the refractive index of the solution plays some role in the sensor response. The LPG was washed with 0.1 M NaOH after each exposure (Figure S5). As the concentration of VA increased, the change in the TS becomes more pronounced, indicating an increase in the amount of VA bound to the nanoMIPs. This behaviour of the TS of the coated LPG fibre is typical of that observed when the RI of the sensitive layer increases¹⁵⁻¹⁸. The resonance band at ca. 670 nm, which is coupled to the linearly polarized 18th cladding mode (LP_{018}), exhibits blue shifts of 0.22, 0.40, 0.60 and 0.88 nm for the 0.01, 0.1, 10 and 700 μM VA concentrations, respectively. The transmission intensity of the resonance band at ca. 833 nm, corresponding to coupling to the LP_{019} modes, decreases for 2.85, 4.93, 11.96 and 15.63 % for 0.01, 0.1, 10 and 700 μM VA concentrations, respectively, Figure 3a. The sensor response starts to saturate at a concentration of VA of 700 μM , indicating the specific nature of VA binding, Figure 3b. The main focus of the sensor characterisation was on concentrations lower than the physiological range (10 nM), demonstrating that this approach could be used to develop a sensor with sensitivity that would need dilutions of real samples before testing. This approach would have the effect of reducing interferences when testing biological samples like plasma.

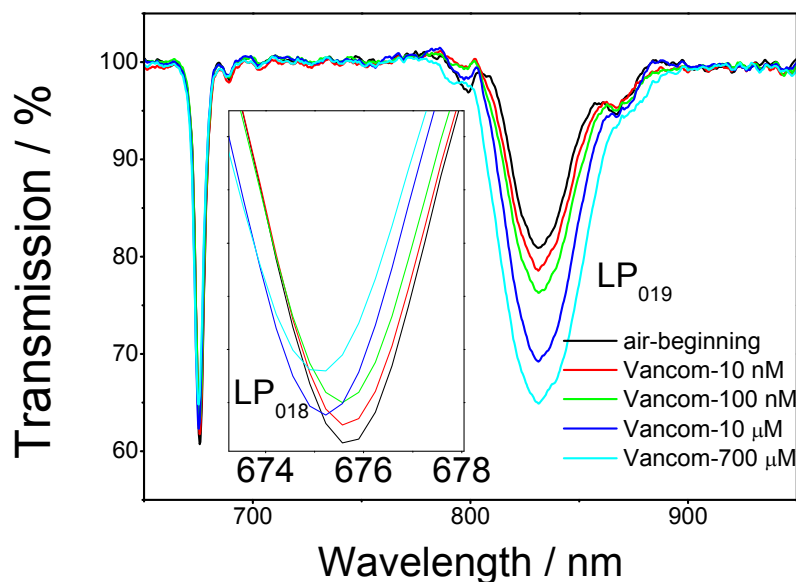

(a)

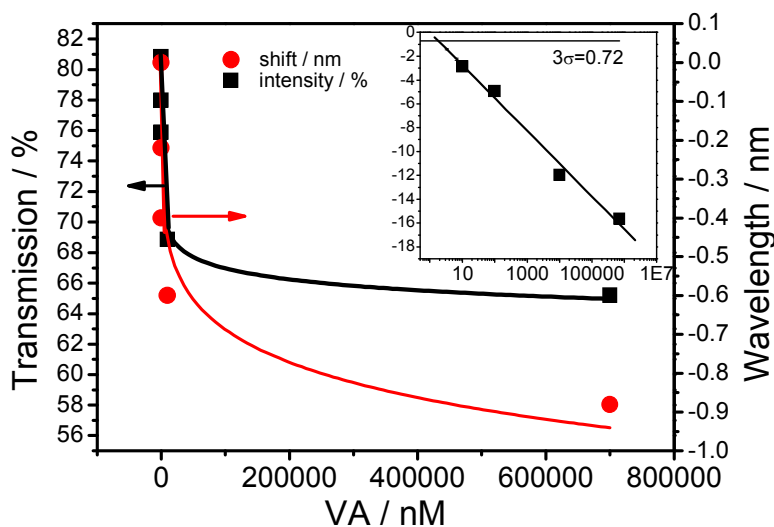

(b)

Figure 3. (a), TS of the nano-MIP coated LPG measured in air after exposure to VA concentrations ranging from 10 nM to 700 μ M; (b), Dependence of the transmission at the centre of the resonance band corresponding to coupling to the LP₀₁₉ mode (square) and wavelength shift of the resonance band corresponding to coupling to the LP₀₁₈ mode (circle) on the concentration of VA. The red and black lines are fits using the Langmuir adsorption isotherm. The inset shows the logarithmic dependence of transmission at the centre of the resonance band corresponding to coupling to the LP₀₁₉ mode on VA concentration.

When the nanoMIP-modified LPG was regenerated with NaOH (0.1 M) the signal returned to its original value, indicating total removal of VA from the nanoMIPs, Figure S5. The binding of VA to the nanoMIPs was fitted with a Langmuir model using the standard package available in Origin software (Figure 3b and S6). The binding constant of VA to the nanoMIPs film, calculated using a Scatchard-Rosenthal plot in accordance with the Eq 2 (Figure S5), was $4.3 \pm 0.01 \times 10^{-8} \text{ M}^{27}$.

$$\frac{B_{max}}{B} = K_d \frac{1}{c} + 1, \quad (2)$$

where B_{max} is the maximum amount of VA bound (sensor response at highest concentration), B is the amount of VA bound at a given concentration (sensor response at a given concentration), K_d is the binding constant and c is the concentration of VA.

The standard deviation, σ , obtained from 5 exposures to blank sample (Figure S6) and 10 μ M of VA, was $\pm 0.24 \%$ and $\pm 0.12 \text{ nm}$ for the transmission and wavelength measurements, respectively. For transmission measurements, the limit of detection of the sensor system was found to be 1.8 nM, determined by calculating the 3σ value²⁷.

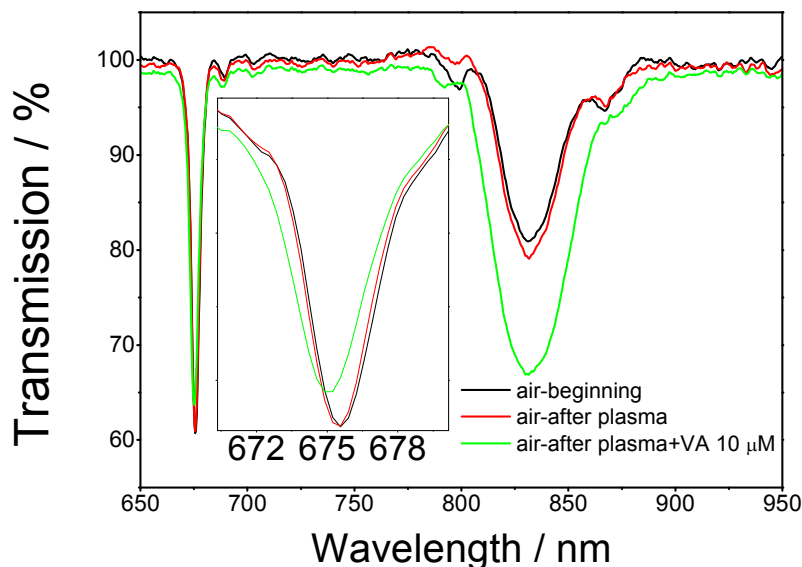


Figure 4. TS of the nano-MIP coated LPG, measured in air before (black line) and after exposure to, porcine plasma (red line) and porcine plasma spiked with 10 μM of VA (green line)

Figure 4 shows the TS measured in air before and after exposure (for 45 minutes) to porcine plasma with and without VA (10 μM). A small sensor response was observed for plasma without VA. The response increased when 10 μM of VA was present in the plasma, Figure 4. These results suggest that the sensor can reliably perform VA detection in a complex medium such as plasma. It should be noted, however, that response to 10 μM of VA was larger when measured in plasma as compared to VA in PBS. The most plausible explanation for this is the effect of the complex medium on the sensor response; this phenomenon could be solved either by further optimisation of the blocking of the particles or by performing an antibiotic calibration curve directly in plasma which should negate the effect of the complex medium. This will be studied in more detail in future work.

3.3 Selectivity test

When the nanoMIPs-modified LPG was exposed to solutions of amoxicillin (610 μM), bleomycin (700 μM) and gentamicin (660 μM), each prepared in PBS, no measurable changes in the central wavelength of the resonance band corresponding to coupling to the LP_{018} mode, nor of the transmission at the centre of the resonance band corresponding to coupling to the LP_{019} mode were observed, revealing the high selectivity of the LPG sensor towards other commonly prescribed antibiotics, (Figure 5).

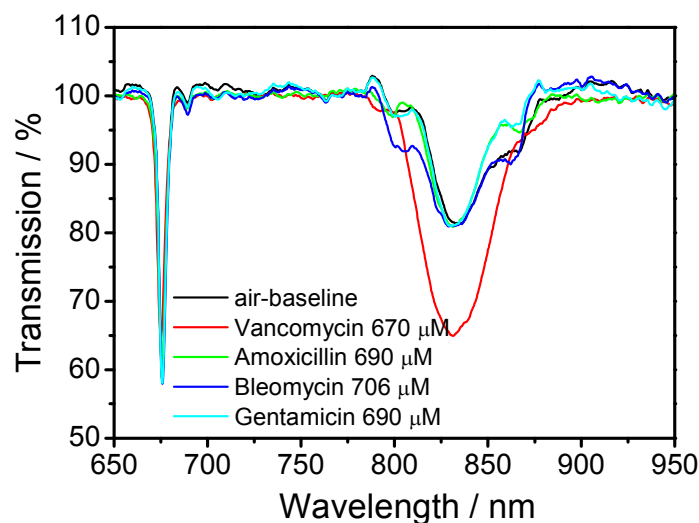


Figure 5. TS of the nano-MIP-coated LPG, measured in air after exposure to, VA (670 μM) (red line), amoxicillin (690 μM) (green line); bleomycin (706 μM) (blue line) and gentamicin (690 μM) (magenta line).

Conclusions

In conclusion, molecularly imprinted polymer nanoparticles specific for VA were successfully deposited for the first time onto an optical fibre long period grating. The sensor demonstrated high sensitivity (10 nM with $4.3 \pm 0.01 \times 10^8 \text{ M}^{-1}$ binding constant) to VA and selectivity over other antibiotics such as amoxicillin, bleomycin and gentamicin. Successful detection of VA in a complex biological matrix, porcine plasma was also demonstrated. The LPG sensor based on molecular imprinted nanoparticles presented here is a promising tool for detection of antibiotics in biological fluids. In addition, the generic nature of both the LPG sensor and the nanoMIP prepared by solid-phase synthesis suggests that by immobilizing different nanoMIPs (produced against a different analyte), low cost and easy to use optical fibre sensors can be produced for applications in a variety of fields, from medical and environmental to food and industry.

Acknowledgment

The authors thank The Wellcome Trust (UK) for the financial support through the granting of a Translational Award and the EPSRC Platform Grant (EP/H02252X/1).

References

1 H.M.R. Goncalves, A.J. Duarte, F. Davis and S.P.J. Higson, *Analytica Chimica Acta*, 2012, **735**, 90.

- 1
2 2 M. Consales, S. Campopiano, A. Cutolo, M. Penza, P. Aversa, G. Cassano, M. Giordano and A.
3 Cusano, *Measurement Science and Technology*, 2006, **17**, 1220.
4
5
6 3 S.-W. Lee, S. Korposh, R. Selyanchyn and T. Kunitake, in: *Handbook of Molecular Imprinting:*
7 *Advanced Sensor Applications*, ed. S.-W. Lee and T. Kunitake, Pan Stanford Publishing Pte Ltd, 2012, ch.
8 1, pp. 1-64.
9
10 4 M.J. Whitcombe, I. Chianella, L. Larcombe, S.A. Piletsky, J. Noble, R. Porter and A. Horgan, *Chemical*
11 *Society Reviews*, 2011, **40**, 1547.
12
13 5 C. Malitesta, E. Mazzotta, R.A. Picca, A. Poma, I. Chianella and S.A. Piletsky, *Analytical and*
14 *Bioanalytical Chemistry*, 2011, **402**, 1827.
15
16
17 6 G. Diaz-Diaz, D. Antuna- Jimenez, M.C. Blanco-Lopez, M.J. Lobo-Castanon, A.J. Miranda-Ordieres
18 and P. Tunon-Blanco, *Trends in Analytical Chemistry*, 2012, **33**, 68.
19
20 7 Y. Uludag, S.A. Piletsky, A.P.F. Turner and M.A. Cooper, *FEBS Journal*, 2007, **274**, 5471.
21
22 8 A. Poma, A. Guerreiro, M. J. Whitcombe, E. V. Piletska , A. P. F. Turner and S. A. Piletsky, *Advanced*
23 *Functional Materials*, 2013, **23**, 2821.
24
25
26 9 E. Moczko, A. Poma, A. Guerreiro, I. Perez de Vargas Sansalvador, S. Caygill, F. Canfarotta, M.J.
27 Whitcombe and S. Piletsky, *Nanoscale*, 2013, **5**, 3733.
28
29 10 I. Chianella, A. Guerreiro, E. Moczko, J. S. Caygill, E. V. Piletska, I. M. Perez De Vargas
30 Sansalvador, M. J. Whitcombe and S. A. Piletsky *Anal. Chem.* 2013, **85**, 8462.
31
32 11 M. Rybak, B. Lomaestro, J.C. Rotschafer, R. Moellering, W. Craig, M. Billeter, J.R. Dalovisio and
33 D.P. Levine, *Am J Health-Syst Pharm.*, 2009, **66**, 82.
34
35
36 12 J. Truong, B.J. Levkovich and A.A. Padiglione, *Internal Medicine Journal*, 2012, **42**, 23.
37
38 13 M.J. de Jesus Valle, F. Gonzalez Lopez, A. Sanchez Navarro, *Journal of Pharmaceutical and*
39 *Biomedical Analysis*, 2008, **48**, 835.
40
41 14 K. A. Rodvold, S. M. Erdman and R. D. Pryka, in: *Therapeutic drug monitoring*, ed. Schumacher G.
42 E., Appleton and Lange: Norwalk, CT, 1995, pp. 587–632.
43
44 15 S. A. Simons, A. R. Molinelli, K. Sobhani, P. M. Rainey and A. N. Hoofnagle, *Clinical Chemistry*,
45 2009, **55**, 578.
46
47 16 S. Korposh, S.-W. Lee, S. W. James and R. P. Tatam, *Meas. Sci. Technol.*, 2011, **22**, 075208 (10 p).
48
49 17 S. Korposh, S. W. James, S. W. Lee, S. Topliss, S. C. Cheung, W. J. Batty and R. P. Tatam, *Optics*
50 *Express*, 2010, **18**, 13227.
51
52 18 T. Wang, S. Korposh, R. Wong, S. James, R. Tatam and S. W. Lee, *Chem. Lett.*, 2012, **41**, 1297.
53
54 19 S. Korposh, T. Wang, S. James, R. Tatam and S. W. Lee, *Sens. Act. B.*, 2012, **173**, 300.
55
56 20 R. Falciai, A.G. Mignani and A. Vannini, *Sens. Actuators B.*, 2001, **74**, 74.
57
58
59
60

-
- 1
2
3 21 R. Verma and B.D. Gupta, *Sens. Actuators B.*, 2013, **177**, 279.
4
5
6 22 N. Cennamo, G. D'Agostino, R. Galatus, L. Bibbo', and M.Pesavento, L. Zeni, *Sens. Actuators B.*,
7 2013, DOI: 10.1016/j.snb.2013.07005.
8
9 23 T.H. Nguyen, S.A. Hardwick, S. Tong, K.T.U. Grattan, *IEEE Sensors Journal*, 2012, **12**, 255.
10
11 24 K. Fujiwara, Y. Yoshizaki, M. Shin, T. Miyazaki, T.Saita, and S.Nagata, *Antimicrobial Agents*
12 *Chemotherapy*, 2012, **56**, 5883.
13
14 25 Y. Hoshino, T. Urakami, T. Kodama, H. Koide, N. Oku, Y. Okahata, K. J. Shea, *Small*, 2009, **5**, 1562.
15
16 26 S.C. Cheung, S.M. Topliss, S. W. James and R. P. Tatam, *Journal of the Optical Society of America B*,
17 2008, **25**, 897.
18
19 27 A. Bossi, S. A. Piletsky, E. V. Piletska, P. G. Righetti and A. P. F. Turner *Anal. Chem.* 2001, **73**,
20 5281.
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Table of contents entry

Selective vancomycin detection using long period grating fibres functionalised with molecularly imprinted polymer nanoparticles

Sergiy Korposh¹, Iva Chianella², Antonio Guerreiro², Sarah Caygill², Sergey Piletsky², Stephen W. James¹, Ralph P. Tatam¹

¹Department of Engineering Photonics, School of Engineering, Cranfield University, Cranfield, Bedfordshire, MK43 0AL, UK

²Cranfield Health, Cranfield University, Cranfield, Bedfordshire, MK43 0AL, UK

Molecularly imprinted polymer nanoparticles (nanoMIPs) were deposited onto an optical fibre long period grating (LPG) sensor for the first time with aim of the specific detection of antibiotics. The operation of the sensor is based on the measurement of changes in refractive index induced by the interaction of nanoMIPs deposited onto the cladding of the LPG with free vancomycin (VA).

