

# Chemical Science

rsc.li/chemical-science



ISSN 2041-6539



ROYAL SOCIETY  
OF CHEMISTRY

**EDGE ARTICLE**

Yi Lu *et al.*

Translating molecular detections into a simple temperature test using a target-responsive smart thermometer

Cite this: *Chem. Sci.*, 2018, 9, 3906

# Translating molecular detections into a simple temperature test using a target-responsive smart thermometer†

Jingjing Zhang,  Hang Xing  and Yi Lu \*

While it has been well recognized that affordable and pocket-size devices play a major role in environmental monitoring, food safety and medical diagnostics, it often takes a tremendous amount of resources to develop such devices. Devices that have been developed are often dedicated devices that can detect only one or a few targets. To overcome these limitations, we herein report a novel target-responsive smart thermometer for translating molecular detection into a temperature test. The sensor system consists of a functional DNA–phospholipase A<sub>2</sub> (PLA<sub>2</sub>) enzyme conjugate, a liposome-encapsulated NIR dye, and a thermometer interfaced with a NIR-laser device. The sensing principle is based on the target-induced release of PLA<sub>2</sub> from the DNA–enzyme conjugate, which catalyzes the hydrolysis of liposome to release the NIR dye inside the liposome. Upon NIR-laser irradiation, the released dye can convert excitation energy into heat, producing a temperature increase in solution, which is detectable using a thermometer. Considering the low cost and facile incorporation of the system with suitable functional DNAs to recognize many targets, the system demonstrated here makes the thermometer an affordable and pocket-size meter for the detection and quantification of a wide range of targets.

Received 15th December 2017

Accepted 7th March 2018

DOI: 10.1039/c7sc05325h

rsc.li/chemical-science

## Introduction

The ability to detect and quantify a broad range of targets at home or in the field is very important for applications such as environmental monitoring, food safety and medical diagnostics.<sup>1–5</sup> In order to carry out such measurements quantitatively, portable devices such as fluorimeters are often required, and, given the wide availability of smartphones, devices that can interface with smartphones are also preferred.<sup>6,7</sup> Despite the progress made so far, most portable devices still require a fair amount of resources for their development and manufacture, making the devices unaffordable to most users at home. In addition, most of these devices are not small enough to be placed in pockets for convenient and frequent use. To overcome these limitations, we and others have taken advantage of the widely available pocket-sized personal glucose meters (PGMs) and developed novel methods to convert binding of non-glucose targets by functional DNAs (*e.g.*, aptamers and DNazymes) into glucose so that anyone can use the PGM for the quantification of a wide range of targets from heavy metal ions to organic toxins, cancers and pathogens.<sup>8–12</sup> Even though millions of diabetics have PGMs, most other people do not possess PGMs at

home. Therefore, there is a need to search for other portable devices that are even more widely available and cheaper.<sup>13,14</sup>

The thermometer is arguably the most widely available, smallest and cheapest quantitative device for measurements. The determination of the temperature is one of the most important analytical methods in environmental monitoring and medical diagnostics.<sup>15–17</sup> As a result, various thermometers were developed for scientific research,<sup>18,19</sup> environmental monitoring,<sup>20,21</sup> and personal healthcare.<sup>22</sup> However, most of the commercialized thermometers are still limited in that they can only detect a single “target”, temperature.

A major challenge in using a thermometer to measure a broad range of targets beyond temperatures is to find a method that can link the binding of any targets with a change of temperature so that one can use any thermometer to detect the target and measure its concentrations. Conventional calorimetric biosensors utilize enzymatic reactions to generate heat and correlate it with the concentration of the substrate.<sup>23–28</sup> Most of the methods, however, are either time-consuming, labor-intensive, high cost, or require highly technical expertise and sophisticated instrumentation, which limits their application for field work or POC testing.<sup>29,30</sup> To overcome the limitation, integrated sensors based on the photo-thermal effect of hemoglobin have been described, but their sensitivity is low, due to the relatively low thermal generation efficiency of hemoglobin.<sup>31–33</sup> While the exothermic chip sensor, based on an aptamer-modified hydrogel to modulate the capillary fluid flow rate to control the heat produced by the exothermic reagent (*e.g.*

Department of Chemistry, University of Illinois at Urbana-Champaign, Urbana, IL 61801, USA. E-mail: yi-lu@illinois.edu

† Electronic supplementary information (ESI) available: Details of the experimental procedures and other figures. See DOI: 10.1039/c7sc05325h




NaOH) dissolution, can provide high sensitivity,<sup>34</sup> its performance is often affected by the endogenous fluid viscosity, making it unsuitable for the analysis of biological samples (e.g. blood or serum). Recently, a nanoparticle-mediated photo-thermal bioassay using a thermometer as the signal reader has been developed for detecting biomolecules (e.g. Prostate-specific antigen) using antibodies.<sup>35</sup> However, antibodies don't have good sensitivity and selectivity when applied for detecting small molecule targets (e.g. metal ions and small molecule drugs). Therefore, it is still a challenge to integrate thermometers with a convenient and highly sensitive sensing system for quantitative bioanalysis of a wide range of targets.

In this paper, we take advantage of the excellent photo-thermal properties of indocyanine green (ICG) that is encapsulated in liposomes and target-responsive functional DNA (aptamer or DNAzyme) conjugated to phospholipase A<sub>2</sub> (PLA<sub>2</sub>) to provide a quantitative link between the target and the temperature readout of a thermometer for on-site and real-time detections. Our sensor system includes several key features: first, a biotin-DNA immobilized onto magnetic beads (MBs) by means of streptavidin–biotin binding, and the DNA–PLA<sub>2</sub> conjugate synthesized *via* the maleimide–thiol reaction, both of which hybridize with the target-responsive functional DNAs (e.g. structure-switching aptamer or RNA-cleaving DNAzyme) to form a DNA sandwich structure; this design can provide a general platform for the recognition of a wide range of targets. Second, ICG is the only near-infrared (NIR) photosensitizer dye approved by the United States Food and Drug Administration (FDA) for clinical use and has a wide range of applications in imaging and photo-thermal therapy,<sup>36,37</sup> because it can effectively convert NIR laser light into heat. Third, liposomes are spherical lipid vesicles having a phospholipid bi-layered membrane structure,<sup>38</sup> which have been widely used as carriers of different signaling tracers with high carrying capacity.<sup>39–42</sup> Finally, the encapsulated ICG can be easily released by PLA<sub>2</sub>, which is a superfamily of enzymes that degrade phospholipids by cleaving the sn-2 acyl ester bond of glycerol phospholipids to produce free fatty acids and lysolipids.<sup>43,44</sup> For this reason, PLA<sub>2</sub> could provide a link between the target concentration and the temperature readout.

## Results and discussion

The sensor reported in this work, called target-responsive smart thermometer (TRESTM), is comprised of three components (Scheme 1): a functional DNA conjugated to the PLA<sub>2</sub> enzyme at its 5' end and immobilized onto magnetic beads (MBs) at its 3' end, which establishes the relationship between target concentration and enzyme concentration based on the target-induced release of the DNA–PLA<sub>2</sub> conjugate; liposome-encapsulated ICG, which acts as a signal amplifier; and a NIR-laser integrated thermometer, which is used as a downstream transducer for temperature signal output. The binding of a target by the functional DNA can result in the release of PLA<sub>2</sub> from the functional DNA–PLA<sub>2</sub> conjugates that are immobilized on the MBs, and the released PLA<sub>2</sub> then catalyzes the hydrolysis of the liposome to release the ICG from its core. Upon NIR-laser

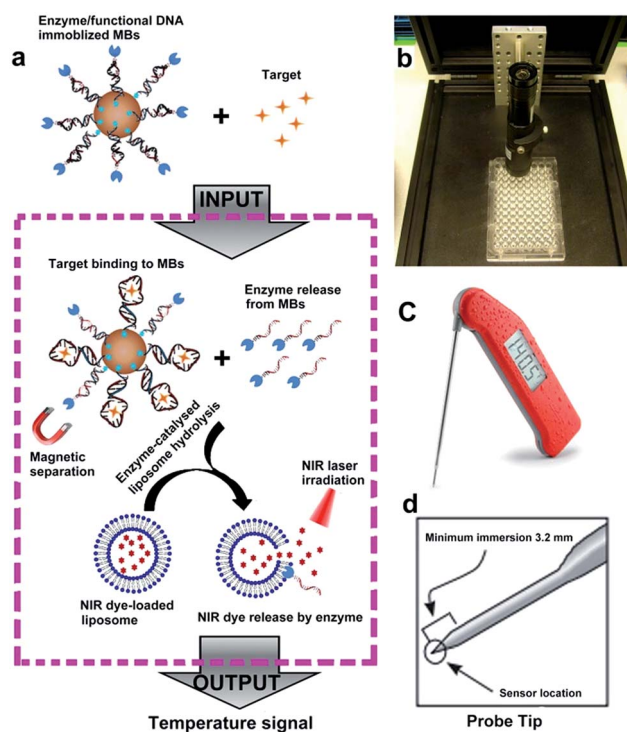

**Scheme 1** (a) Schematic view of the design and working mechanism of the sensor based on a functional DNA and thermometer. (b) Photo of the photothermal chamber including a NIR laser pointer, and a 96-well colorless plate. (c) Photo of the super-fast Thermapen with 3 second readings that were used to detect the temperature change during laser irradiation. (d) Probe tip with a minimum immersion of 3.2 mm, which could measure the solution temperature in a small volume (180  $\mu$ L).

light irradiation in a photo-thermal chamber (Scheme 1b), the released ICG can convert the light excitation energy into heat, producing a temperature increase in solution, which is detectable using a super-fast Thermapen (Scheme 1c and d). Since the output temperature signal is related to the presence and concentration of the released ICG in solution, which in turn depends on the presence and concentration of the released PLA<sub>2</sub> by the target, the presence and concentration of the target can be determined by monitoring the temperature change in the system. Furthermore, by taking advantage of the enormous amplification afforded by liposome-encapsulated ICG, the system can greatly enhance the high sensitivity of the novel thermometer transducer system, and hence lead to an ultra-sensitive thermosensor.

Fig. S1a† illustrates the synthetic approach to prepare the DNA–PLA<sub>2</sub> conjugate using the maleimide–thiol reaction.<sup>45</sup> The UV-vis absorption spectrum of the purified DNA–PLA<sub>2</sub> conjugate overlays well with the sum of the spectra of its two components, DNA and PLA<sub>2</sub> (Fig. S1b†), suggesting successful conjugation. The successful conjugation has also been confirmed by SDS-PAGE, followed by fluorescence and photographic imaging. In this experiment, the thiolated DNA was modified with fluorescein so that the free DNA and DNA–PLA<sub>2</sub> conjugate could be fluorescently imaged (Fig. S1c†), while the free PLA<sub>2</sub> was stained with Coomassie Brilliant Blue (Fig. S1d†).



Another important component of our thermometer system is the liposome that contains ICG, which can be prepared by the film hydration and extrusion method to sequester a large amount of the ICG dye for signal amplification.<sup>46–48</sup> The UV-vis absorption spectrum of liposome-ICG shows a significant red shift (by 22 nm) from that of free ICG (Fig. 1a), suggesting that ICG has been integrated into the lipid bilayers of the liposome after encapsulation, as reported previously.<sup>49</sup> The dynamic light scattering (DLS) spectrum suggests an average hydration diameter of  $\sim 155$  nm with a uniform distribution (Fig. S2†). After incubating the liposome-ICG with PLA<sub>2</sub> for 1 h, the average hydration diameter increased to about 221 nm, indicating the hydrolysis of liposome-ICG by PLA<sub>2</sub>. The enzymatic hydrolysis reaction was further analyzed by monitoring the released ICG in the supernatant using UV absorption spectra (Fig. 1b), demonstrating that even subtle changes in PLA<sub>2</sub> concentration (e.g. 5 nM) could release a large amount of the ICG dye, which can be subsequently transduced into an enhanced temperature signal.

To test the ability of the above TRESTM to detect a broad range of targets, we first explored quantitative detection of cocaine using a cocaine aptamer. Cocaine is an addictive drug, and serves as a representative model target for testing new aptamer-based analytical techniques due to unmet diagnostic needs.<sup>50,51</sup> As shown in Fig. 2a, a DNA sandwich structure was assembled on MBs by connecting the DNA-PLA<sub>2</sub> conjugate to a biotinylated capture DNA (biotin-DNA) through simultaneous hybridization with the cocaine aptamer. In the presence of cocaine, a target-specific structure switching of the aptamer could cause the disassembly of the DNA sandwich structure.<sup>52</sup> This disassembly process was verified by fluorescence assays using FAM-labeled DNA-PLA<sub>2</sub> conjugates (Fig. 2b). The fluorescence intensity increased as a function of increasing cocaine concentrations, establishing a quantitative relationship between the concentration of the target cocaine and the amount of DNA-PLA<sub>2</sub> released into the solution. The released DNA-PLA<sub>2</sub> conjugates were allowed to catalyze the hydrolysis of the liposome to release the ICG from its core, which converted the light excitation energy into heat, producing a temperature increase in solution that can be measured with a thermometer. To release as much ICG as possible for maximal signal output, the concentration of liposome-ICG, determined using a calibration curve of UV absorbance *versus* ICG concentration (Fig. S3†), was

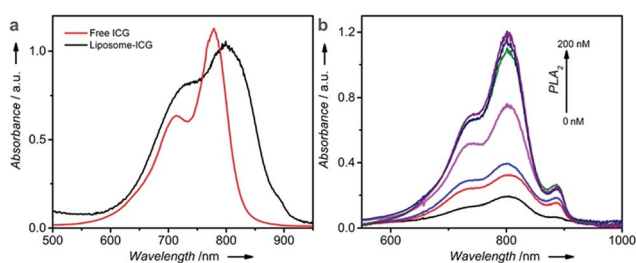


Fig. 1 (a) UV-vis spectra of free ICG and liposome-ICG. (b) UV-vis spectra of the supernatant collected after incubating liposome-ICG with different concentrations of PLA<sub>2</sub> for 2 h. Bottom to top: 0, 5, 10, 20, 50, 100, and 200 nM.

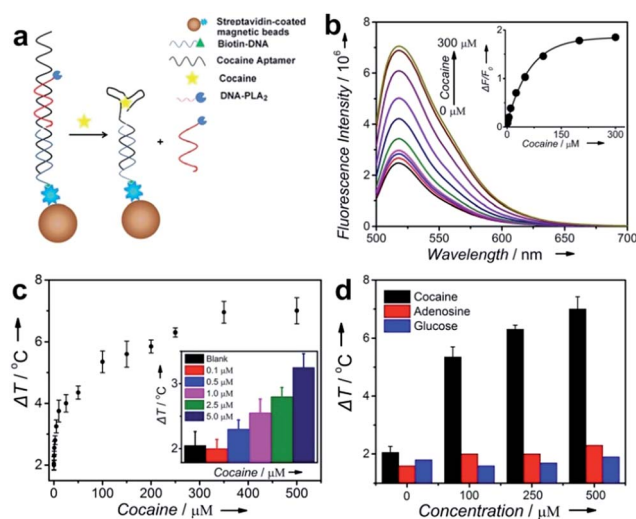


Fig. 2 Design and performance of cocaine detection using the TRESTM system. (a) Cocaine-induced release of immobilized DNA-PLA<sub>2</sub> conjugates. (b) Fluorescence spectra of the release of FAM-labeled DNA-PLA<sub>2</sub> conjugates upon the addition of cocaine at different concentrations. Inset: calibration curve for cocaine detection. (c) Cocaine detection in buffer using the TRESTM. Inset: comparison of the temperature increase at low concentrations of cocaine. (d) Selectivity of cocaine detection using the TRESTM.

chosen as  $0.25 \text{ mg mL}^{-1}$  in subsequent experiments. In addition, to obtain high analytical performance, some important detection parameters, including the time of enzymatic hydrolysis and NIR irradiation, were also optimized (Fig. S4†).

In the absence of cocaine, the temperature increase ( $\Delta T$ ), defined as the temperature change of the supernatant solution before and after the NIR laser irradiation, was  $\sim 2$  °C, which may be due to the nonspecific release of the DNA-PLA<sub>2</sub> conjugate or ICG leakage during centrifugation. In contrast, under the same incubation conditions,  $\Delta T$  increased with the increasing input of cocaine and reached a plateau at  $300 \mu\text{M}$  with temperature increased up to  $7$  °C (Fig. 2c). This observation is in agreement with the fluorescence results, which indicated that all the releasable DNA-PLA<sub>2</sub> conjugates were released at this high concentration of cocaine. This TRESTM exhibited a wide dynamic range from  $0$  to  $500 \mu\text{M}$  and showed a limit of detection of  $3.8 \mu\text{M}$ . This sensitivity is comparable to that of commercial cocaine test kits and other portable meter-based cocaine sensors.<sup>10</sup>

To demonstrate the selectivity of the TRESTM, we further carried out a control experiment with two common biological compounds (adenosine and glucose). Continuous addition of up to  $0.5 \text{ mM}$  adenosine or glucose showed a negligible signal change. In contrast, the temperature response of cocaine at  $100 \mu\text{M}$  was much higher (Fig. 2d). These results indicate that the TRESTM retained the aptamer selectivity with a highly specific response to the target, cocaine.

To test the feasibility of applying the TRESTM sensor in real samples, we explored the detection of cocaine in human serum, one of the most challenging media that contain a variety of proteins and other interfering molecules.<sup>53</sup> By testing 18 serum





- 6 S. Ryu, I. Yoo, S. Song, B. Yoon and J. M. Kim, *J. Am. Chem. Soc.*, 2009, **131**, 3800–3801.
- 7 S. Freddi, L. Sironi, R. D'Antuono, D. Morone, A. Dona, E. Cabrini, L. D'Alfonso, M. Collini, P. Pallavicini, G. Baldi, D. Maggioni and G. Chirico, *Nano Lett.*, 2013, **13**, 2004–2010.
- 8 Y. Xiang and Y. Lu, *Nat. Chem.*, 2011, **3**, 697–703.
- 9 J. J. Zhang, Y. Xiang, M. Wang, A. Basu and Y. Lu, *Angew. Chem., Int. Ed. Engl.*, 2016, **55**, 732–736.
- 10 L. Yan, Z. Zhu, Y. Zou, Y. S. Huang, D. W. Liu, S. S. Jia, D. M. Xu, M. Wu, Y. Zhou, S. Zhou and C. J. Yang, *J. Am. Chem. Soc.*, 2013, **135**, 3748–3751.
- 11 Z. Z. Wang, Z. W. Chen, N. Gao, J. S. Ren and X. G. Qu, *Small*, 2015, **11**, 4970–4975.
- 12 J. Su, J. Xu, Y. Chen, Y. Xiang, R. Yuan and Y. Q. Chai, *Chem. Commun.*, 2012, **48**, 6909–6911.
- 13 K. Tram, P. Kanda, B. J. Salena, S. Y. Huan and Y. F. Li, *Angew. Chem., Int. Ed. Engl.*, 2014, **53**, 12799–12802.
- 14 Z. Zhu, Z. C. Guan, D. Liu, S. S. Jia, J. X. Li, Z. C. Lei, S. C. Lin, T. H. Ji, Z. Q. Tian and C. Y. J. Yang, *Angew. Chem., Int. Ed. Engl.*, 2015, **54**, 10448–10453.
- 15 C. H. Marton, G. S. Haldeman and K. F. Jensen, *Ind. Eng. Chem. Res.*, 2011, **50**, 8468–8475.
- 16 H. F. Arata, Y. Rondelez, H. Noji and H. Fujita, *Anal. Chem.*, 2005, **77**, 4810–4814.
- 17 C. Gota, K. Okabe, T. Funatsu, Y. Harada and S. Uchiyama, *J. Am. Chem. Soc.*, 2009, **131**, 2766–2767.
- 18 D. Zhou, M. Lin, X. Liu, J. Li, Z. L. Chen, D. Yao, H. Z. Sun, H. Zhang and B. Yang, *ACS Nano*, 2013, **7**, 2273–2283.
- 19 Y. J. Cui, H. Xu, Y. F. Yue, Z. Y. Guo, J. C. Yu, Z. X. Chen, J. K. Gao, Y. Yang, G. D. Qian and B. L. Chen, *J. Am. Chem. Soc.*, 2012, **134**, 3979–3982.
- 20 S. Lee, J. H. Lee, M. Kim, J. Kim, M. J. Song, H. I. Jung and W. Lee, *Appl. Phys. Lett.*, 2013, **103**, 143114.
- 21 S. Vermeir, B. M. Nicolai, P. Verboven, P. Van Gerwen, B. Baeten, L. Hoflack, V. Vulsteke and J. Lammertyn, *Anal. Chem.*, 2007, **79**, 6119–6127.
- 22 G. L. Ke, C. M. Wang, Y. Ge, N. F. Zheng, Z. Zhu and C. J. Yang, *J. Am. Chem. Soc.*, 2012, **134**, 18908–18911.
- 23 M. Yakovleva, S. Bhand and B. Danielsson, *Anal. Chim. Acta*, 2013, **766**, 1–12.
- 24 F. E. Torres, M. I. Recht, J. E. Coyle, R. H. Bruce and G. Williams, *Curr. Opin. Struct. Biol.*, 2010, **20**, 598–605.
- 25 P. Paul, M. Hossain and G. S. Kumar, *J. Chem. Thermodyn.*, 2011, **43**, 1036–1043.
- 26 L. Zhang and T. Dong, *J. Micromech. Microeng.*, 2013, **23**, 045011.
- 27 M. Yakovleva, O. Buzas, H. Matsumura, M. Samejima, K. Igarashi, P. O. Larsson, L. Gorton and B. Danielsson, *Biosens. Bioelectron.*, 2012, **31**, 251–256.
- 28 S. Zhou, Y. F. Zhao, M. Mecklenburg, D. J. Yang and B. Xie, *Biosens. Bioelectron.*, 2013, **49**, 99–104.
- 29 Y. H. Choi, M. G. Kim, D. H. Kang, J. Sim, J. Kim and Y. J. Kim, *J. Micromech. Microeng.*, 2012, **22**, 045022.
- 30 L. Zhang, T. Dong, X. Y. Zhao, Z. C. Yang and N. M. M. Pires, *IEEE Eng. Med. Biol.*, 2012, 523–526.
- 31 B. S. Kwak, H. J. Kim, H. O. Kim and H. I. Jung, *Biosens. Bioelectron.*, 2010, **26**, 1679–1683.
- 32 B. S. Kwak, H. O. Kim, J. H. Kim, S. Lee and H. I. Jung, *Biosens. Bioelectron.*, 2012, **35**, 484–488.
- 33 C. Yi, J. H. Lee, B. S. Kwak, M. X. Lin, H. O. Kim and H. I. Jung, *Sens. Actuators, B*, 2014, **191**, 305–312.
- 34 B. B. Gao, H. Liu and Z. Z. Gu, *Lab Chip*, 2016, **16**, 525–531.
- 35 G. Fu, S. T. Sanjay, M. Dou and X. Li, *Nanoscale*, 2016, **8**, 5422–5427.
- 36 A. Hannah, G. Luke, K. Wilson, K. Homan and S. Emelianov, *ACS Nano*, 2014, **8**, 250–259.
- 37 L. Wu, S. T. Fang, S. Shi, J. Z. Deng, B. Liu and L. T. Cai, *Biomacromolecules*, 2013, **14**, 3027–3033.
- 38 D. C. Turner, D. Moshkelani, C. S. Shemesh, D. Luc and H. L. Zhang, *Pharm. Res.*, 2012, **29**, 2092–2103.
- 39 K. Y. Chumbimuni-Torres, J. Wu, C. Clawson, M. Galik, A. Walter, G. U. Flechsig, E. Bakker, L. F. Zhang and J. Wang, *Analyst*, 2010, **135**, 1618–1623.
- 40 C. K. Kim and S. J. Lim, *Liposomes*, 2003, **373**, 260–277.
- 41 S. J. Lim and C. K. Kim, *Anal. Biochem.*, 1997, **247**, 89–95.
- 42 H. G. Nie, S. J. Liu, R. Q. Yu and J. H. Jiang, *Angew. Chem., Int. Ed. Engl.*, 2009, **48**, 9862–9866.
- 43 K. Jorgensen, J. Davidsen and O. G. Mouritsen, *FEBS Lett.*, 2002, **531**, 23–27.
- 44 H. Xing, C. L. Zhang, G. Ruan, J. J. Zhang, K. Hwang and Y. Liu, *Anal. Chem.*, 2016, **88**, 1506–1510.
- 45 A. S. D. S. Indrasekara, B. J. Paladini, D. J. Naczynski, V. Starovoytov, P. V. Moghe and L. Fabris, *Adv. Healthcare Mater.*, 2013, **2**, 1370–1376.
- 46 S. T. Proulx, P. Luciani, S. Derzsi, M. Rinderknecht, V. Mumprecht, J. C. Leroux and M. Detmar, *Cancer Res.*, 2010, **70**, 7053–7062.
- 47 S. K. Cool, B. Geers, S. Roels, S. Stremersch, K. Vanderperren, J. H. Saunders, S. C. De Smedt, J. Demeester and N. N. Sanders, *J. Controlled Release*, 2013, **172**, 885–893.
- 48 F. L. Tansi, R. Ruger, M. Rabenhold, F. Steiniger, A. Fahr, W. A. Kaiser and I. Hilger, *Small*, 2013, **9**, 3659–3669.
- 49 N. Beziere, N. Lozano, A. Nunes, J. Salichs, D. Queiros, K. Kostarelos and V. Ntziachristos, *Biomaterials*, 2015, **37**, 415–424.
- 50 J. S. Swensen, Y. Xiao, B. S. Ferguson, A. A. Lubin, R. Y. Lai, A. J. Heeger, K. W. Plaxco and H. T. Soh, *J. Am. Chem. Soc.*, 2009, **131**, 4262–4266.
- 51 B. R. Baker, R. Y. Lai, M. S. Wood, E. H. Doctor, A. J. Heeger and K. W. Plaxco, *J. Am. Chem. Soc.*, 2006, **128**, 3138–3139.
- 52 J. L. He, Z. S. Wu, H. Zhou, H. Q. Wang, J. H. Jiang, G. L. Shen and R. Q. Yu, *Anal. Chem.*, 2010, **82**, 1358–1364.
- 53 A. X. Zheng, J. Li, J. R. Wang, X. R. Song, G. N. Chen and H. H. Yang, *Chem. Commun.*, 2012, **48**, 3112–3114.
- 54 J. W. Liu, A. K. Brown, X. L. Meng, D. M. Crokek, J. D. Istok, D. B. Watson and Y. Lu, *Proc. Natl. Acad. Sci. U. S. A.*, 2007, **104**, 2056–2061.

